


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121123\
Data File : BF136485.D
Acq On : 11 Dec 2023 12:19
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Dec 06 09:40:27 2023

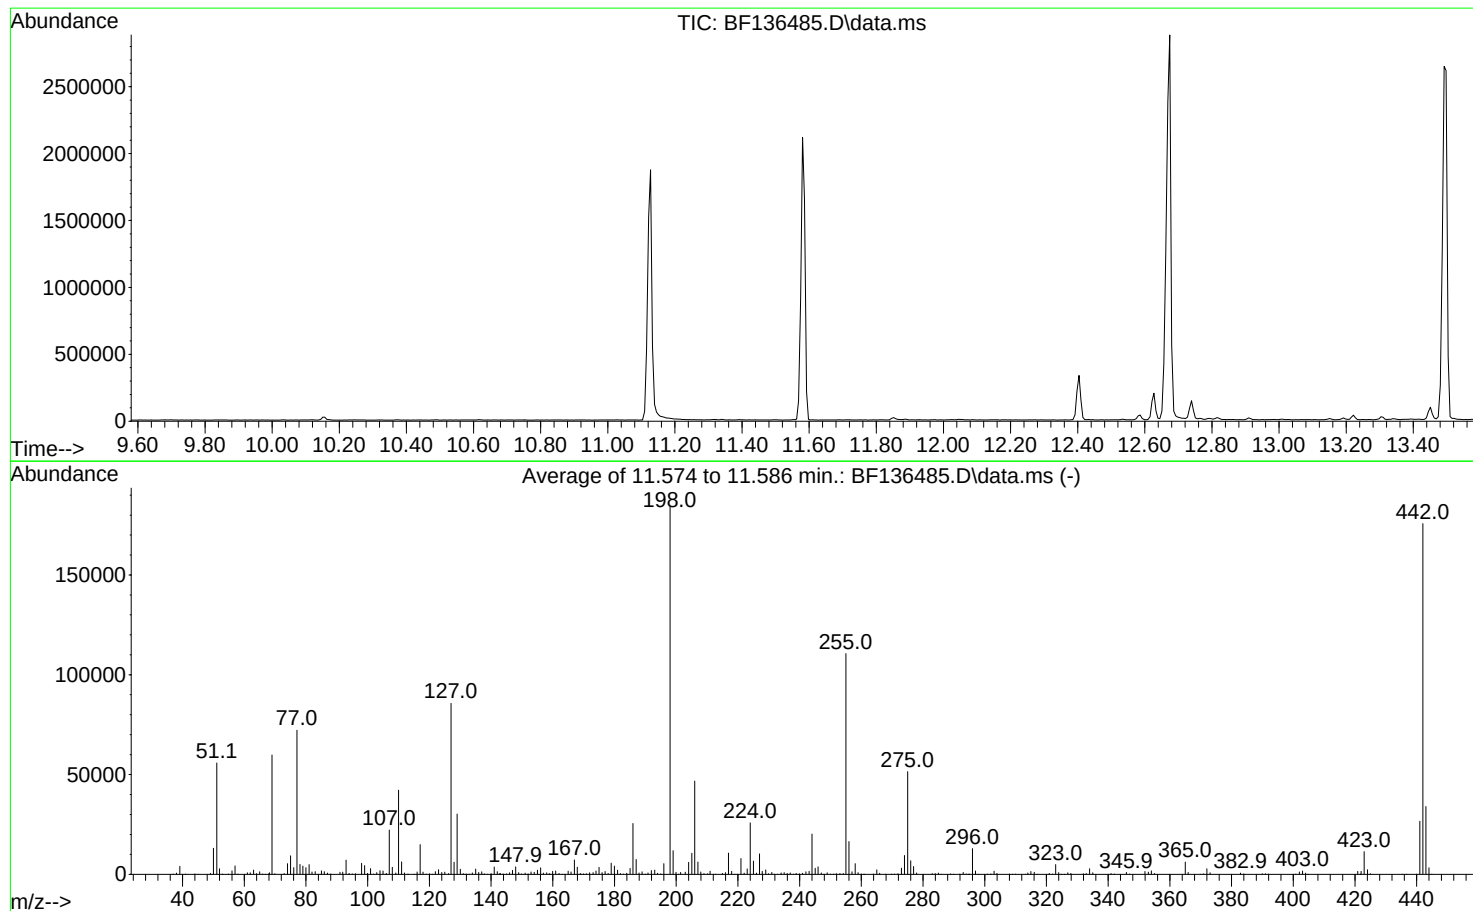




AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.3	55811	PASS
68	69	0.00	2	1.4	809	PASS
69	198	0.00	100	32.4	59784	PASS
70	69	0.00	2	0.5	326	PASS
127	198	10	80	46.5	85701	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	184301	PASS
199	198	5	9	6.4	11858	PASS
275	198	10	60	27.9	51472	PASS
365	198	1	100	3.3	6154	PASS
441	198	0.01	100	14.4	26588	PASS
442	442	50	100	100.0	175744	PASS
443	442	15	24	19.3	34003	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121123\
Data File : BF136485.D
Acq On : 11 Dec 2023 12:19
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 12 00:34:05 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 06 09:40:27 2023
Response via : Initial Calibration

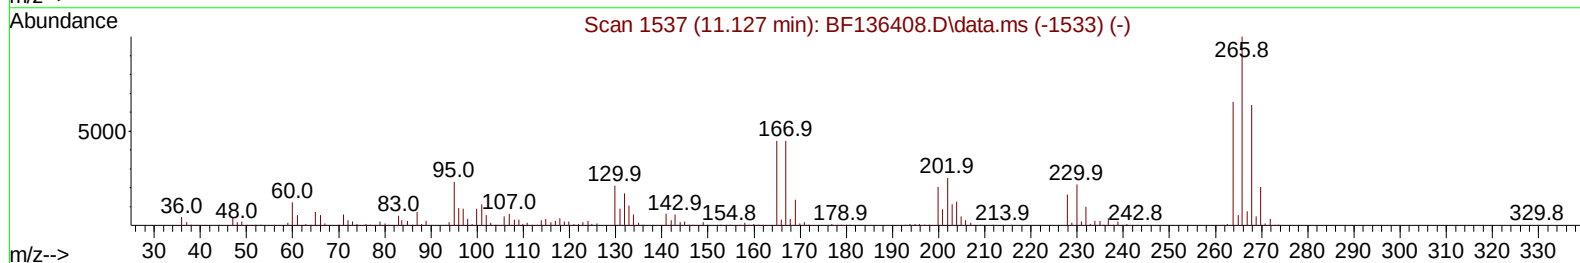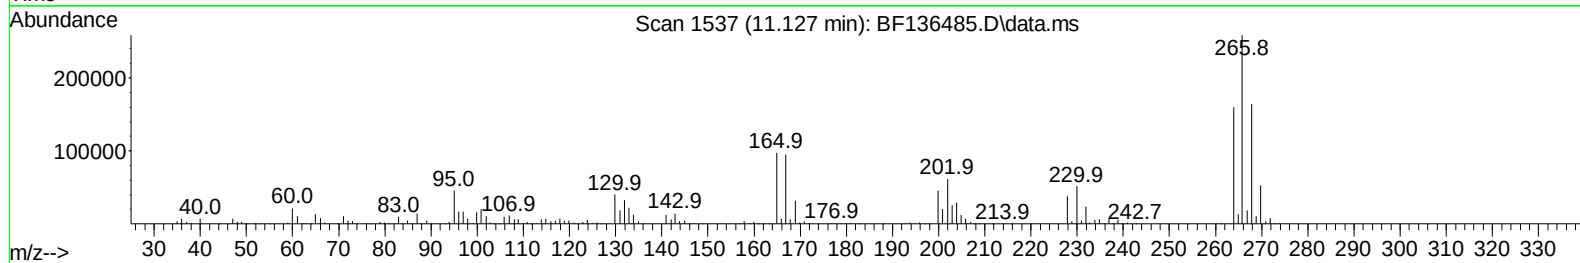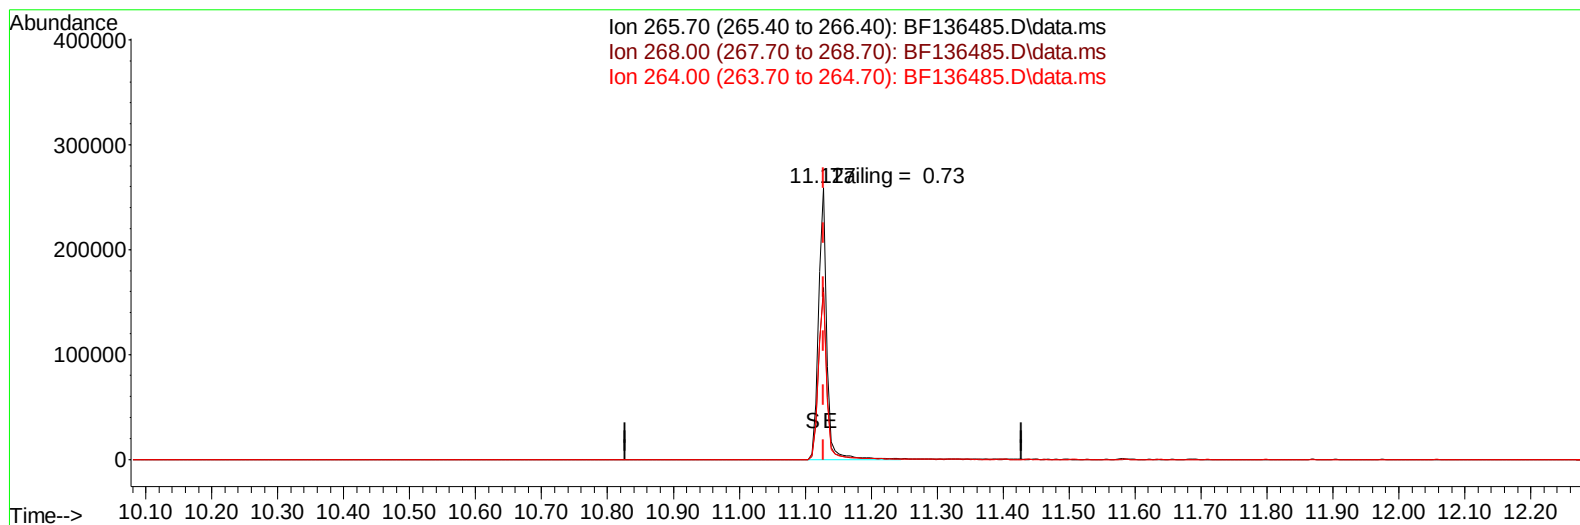

TIC: BF136485.D\data.ms

(70) Pentachlorophenol (C)

11.127min (-0.000) 22410.94 ng




response 227073

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	63.38
264.00	65.30	61.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121123\
Data File : BF136485.D
Acq On : 11 Dec 2023 12:19
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 12 00:34:05 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 06 09:40:27 2023
Response via : Initial Calibration

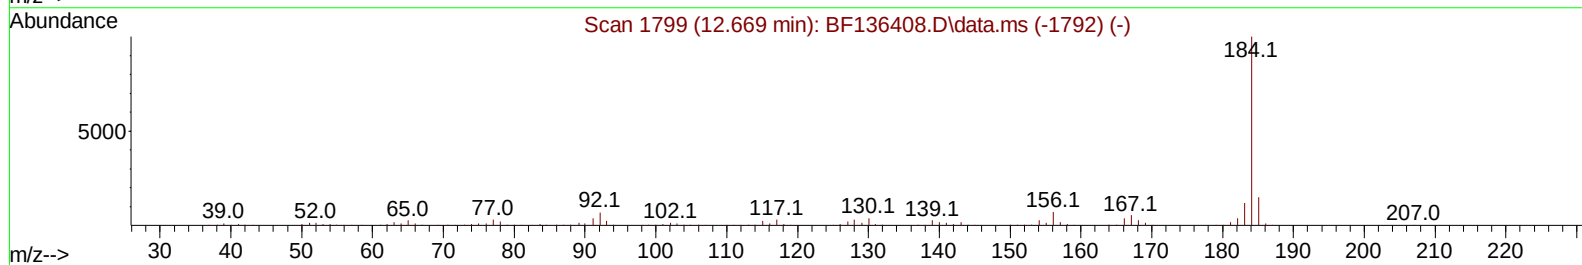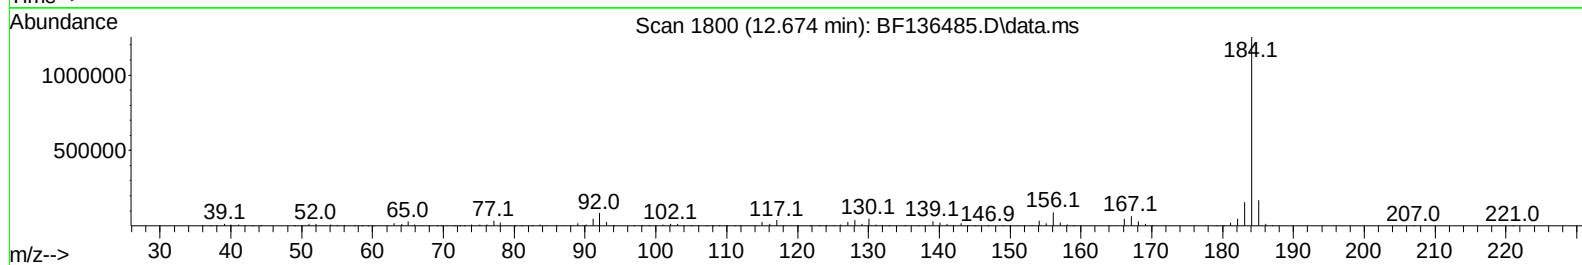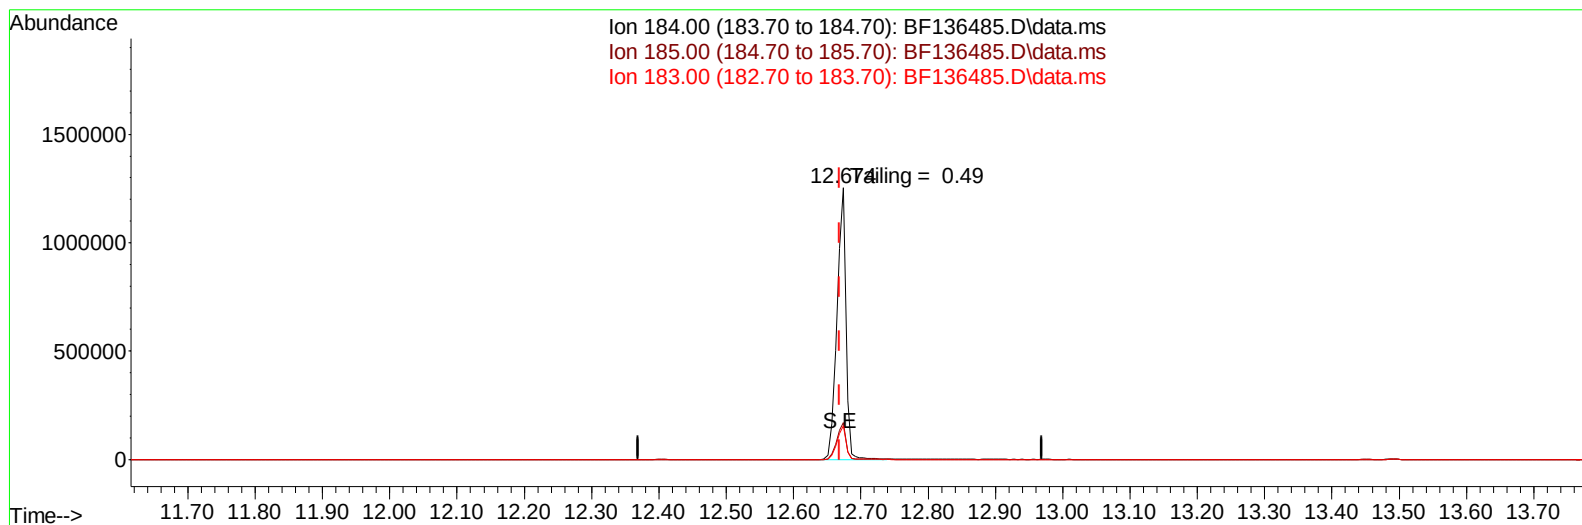

TIC: BF136485.D\data.ms

(77) Benzidine

12.674min (+ 0.005) 1694.10 ng

response 1154853

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	13.49
183.00	11.70	12.41
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/11/2023	BNA_F	<u>BF136485.D</u>
Compound Name	Response	Retention Time
DDT	539804	13.498
DDD	7746	13.221
DDE	389	12.857
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8135	547939	1.48

Instrument :
BNA_F
ClientSampleId :
DFTPP