
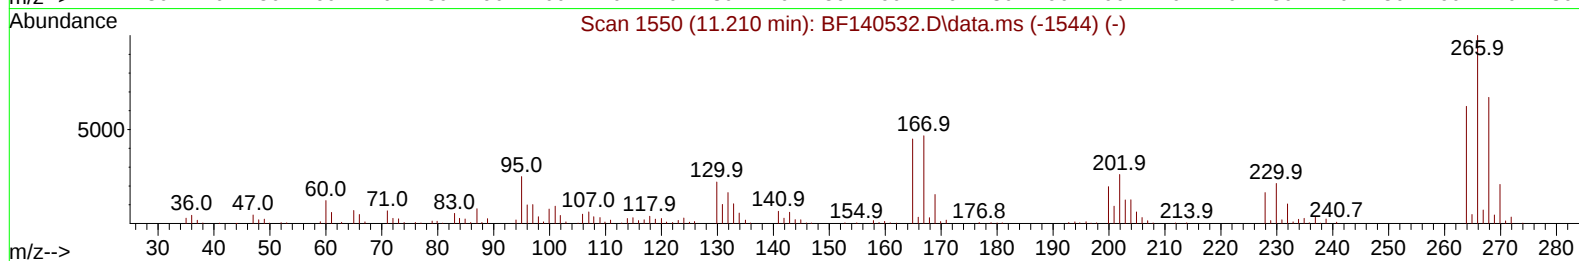
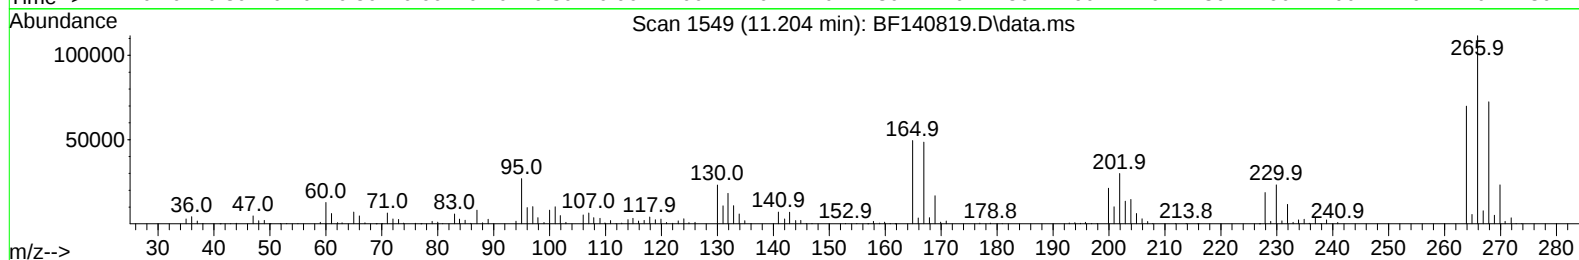


Quant Time: Dec 11 12:47:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 15:23:48 2024
Response via : Initial Calibration

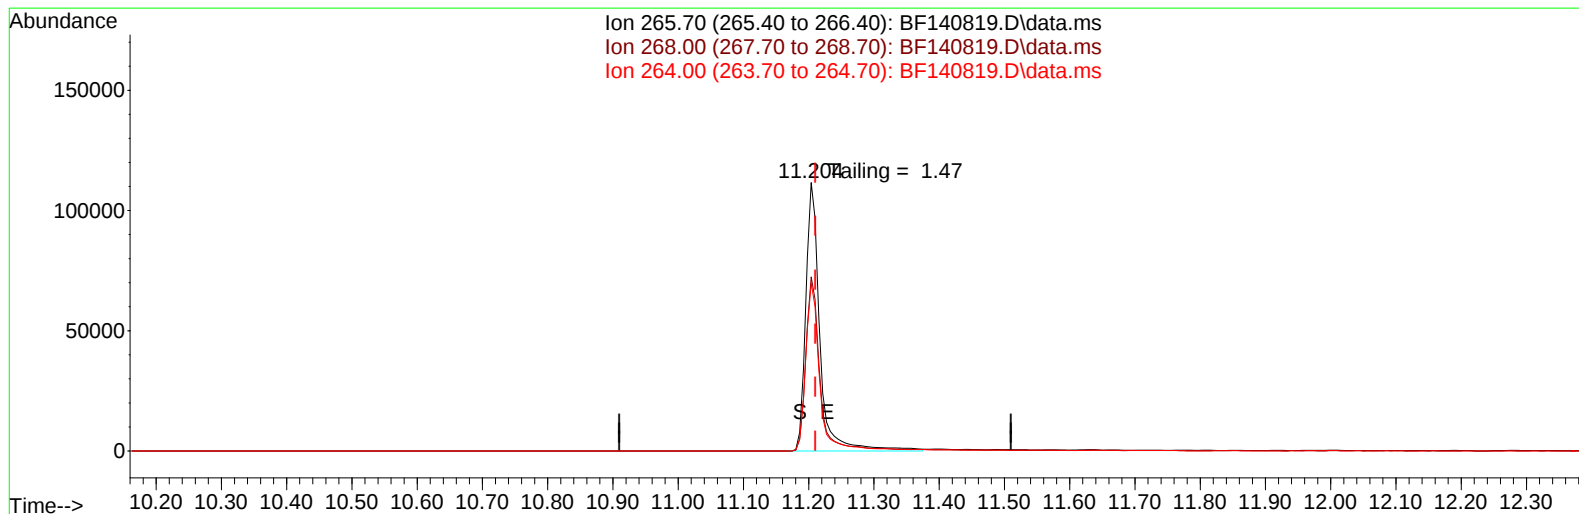

TIC: BF140819.D\data.ms

(70) **Pentachlorophenol (C)**




11.204min (-0.006) 26722.70 ng

response **169561**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.10	64.87
264.00	62.30	62.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121124\
Data File : BF140819.D
Acq On : 11 Dec 2024 10:13
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 11 12:47:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 15:23:48 2024
Response via : Initial Calibration

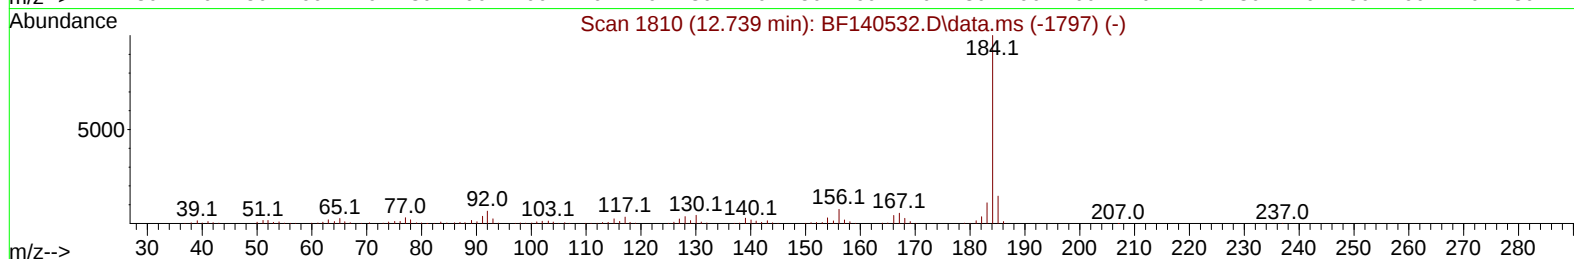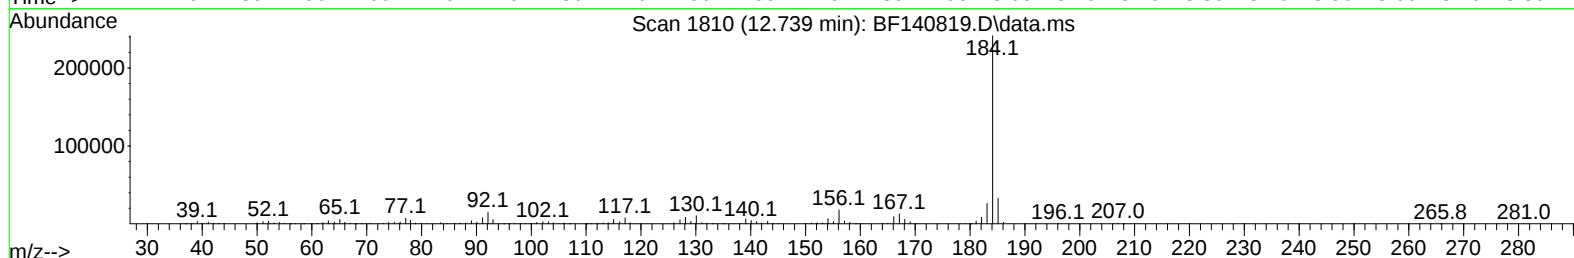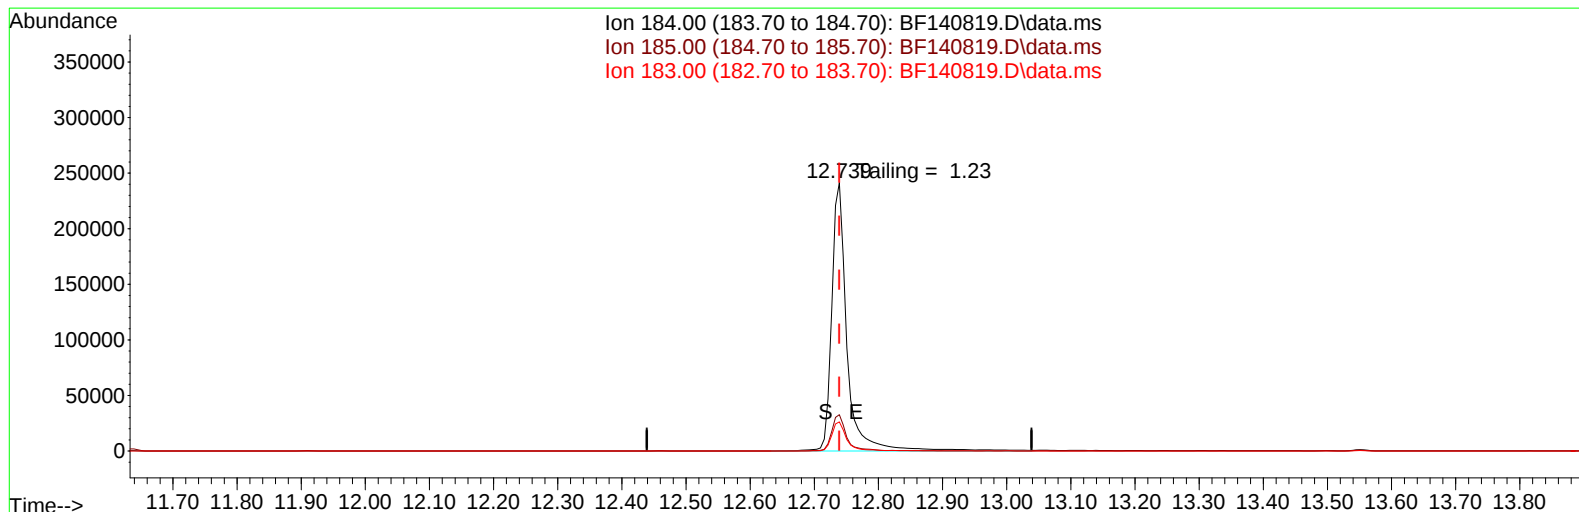

TIC: BF140819.D\data.ms

(77) Benzidine

12.739min (+ 0.000) 12781.12 ng

response **393900**

Ion	Exp%	Act%
-----	------	------

184.00	100.00	100.00
--------	--------	--------

185.00	14.60	13.58
--------	-------	-------

183.00	11.00	10.89
--------	-------	-------

0.00 0.00 0.00