


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121124\
Data File : BF140819.D
Acq On : 11 Dec 2024 10:13
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Nov 21 15:23:48 2024

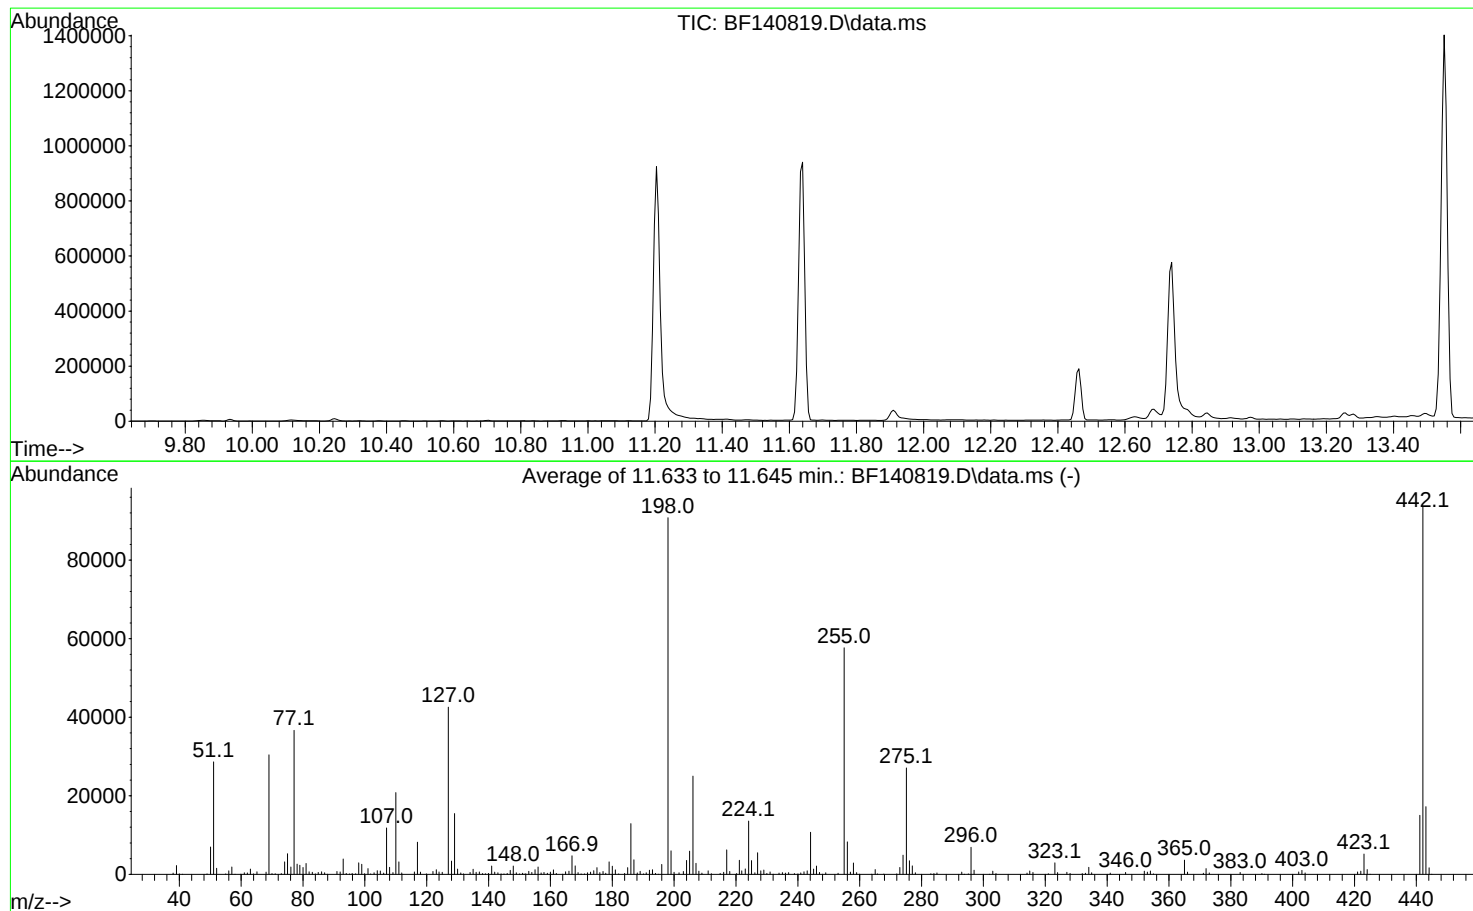

AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.6	28653	PASS
68	69	0.00	2	1.9	569	PASS
69	198	0.00	100	33.5	30425	PASS
70	69	0.00	2	0.7	217	PASS
127	198	10	80	46.9	42563	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	90781	PASS
199	198	5	9	6.6	6010	PASS
275	198	10	60	29.8	27083	PASS
365	198	1	100	4.0	3643	PASS
441	198	0.01	100	16.6	15051	PASS
442	442	50	100	100.0	93648	PASS
443	442	15	24	18.4	17238	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
12/11/2024	BNA_F	<u>BF140819.D</u>
Compound Name	Response	Retention Time
DDT	354374	13.551
DDD	10697	13.257
DDE	1023	12.916
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11720	366094	3.20

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121124\
Data File : BF140819.D
Acq On : 11 Dec 2024 10:13
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 11 12:47:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 15:23:48 2024
Response via : Initial Calibration

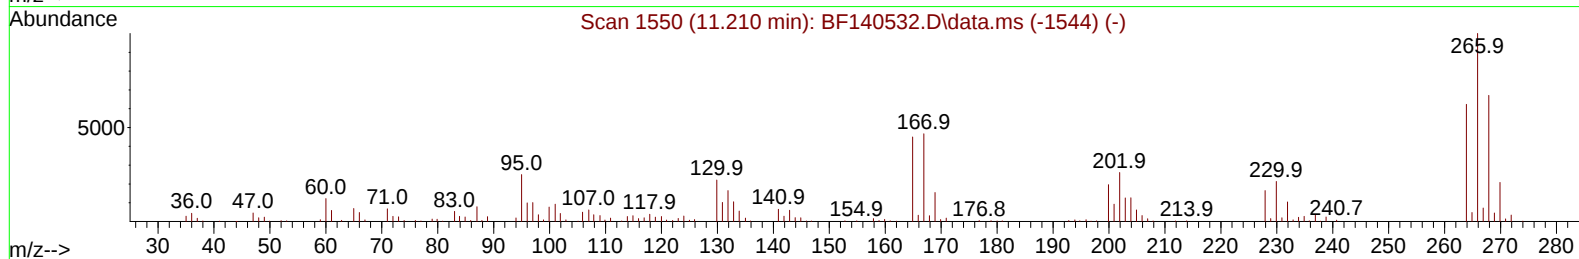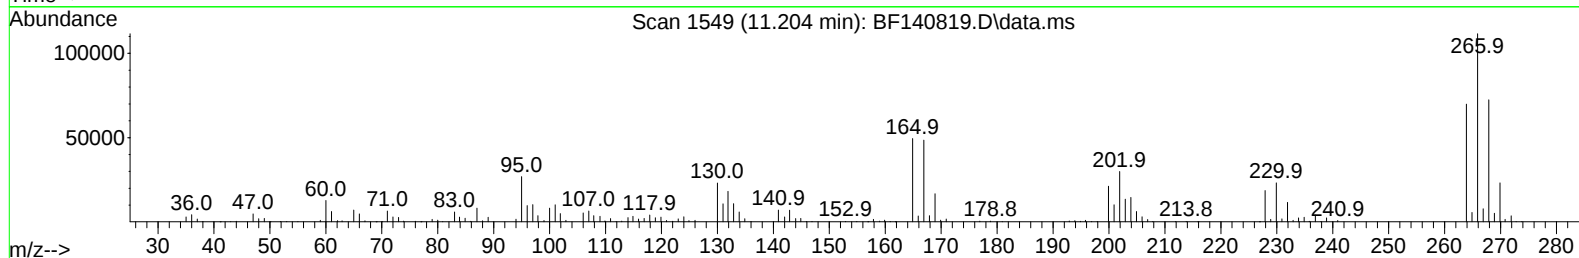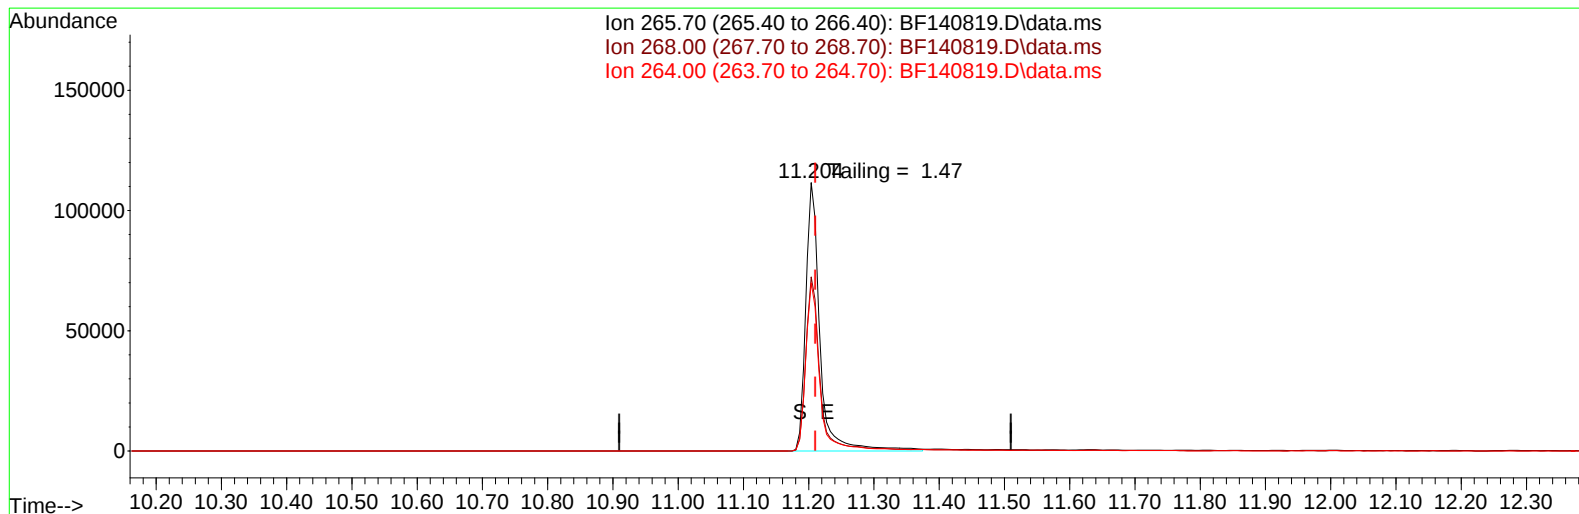

TIC: BF140819.D\data.ms

(70) Pentachlorophenol (C)

11.204min (-0.006) 26722.70 ng




response 169561

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.10	64.87
264.00	62.30	62.65
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121124\  
Data File : BF140819.D  
Acq On    : 11 Dec 2024  10:13  
Operator  : RC/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 11 12:47:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 15:23:48 2024
Response via : Initial Calibration

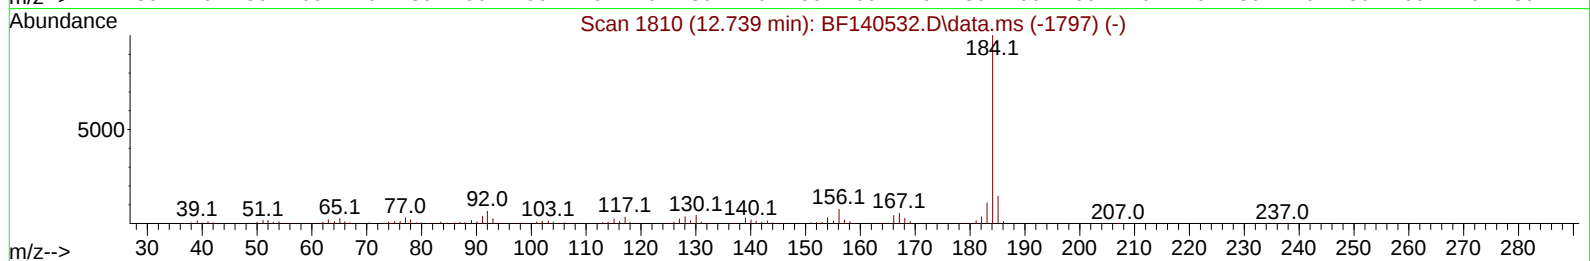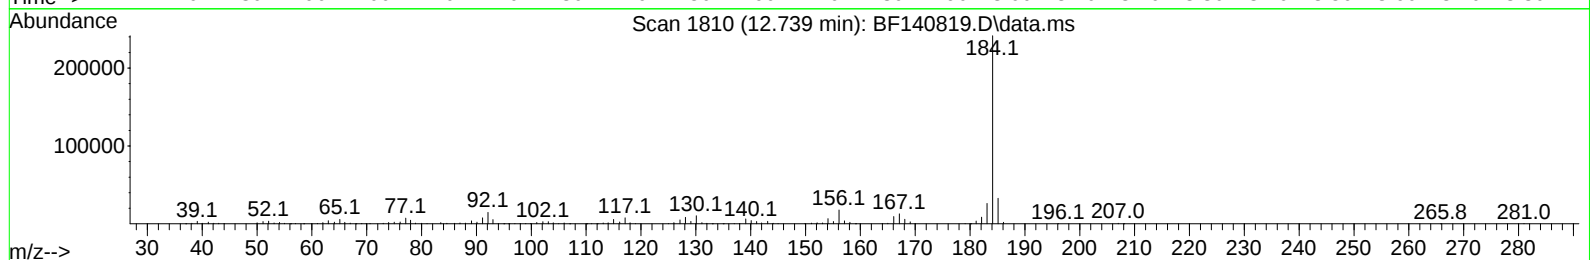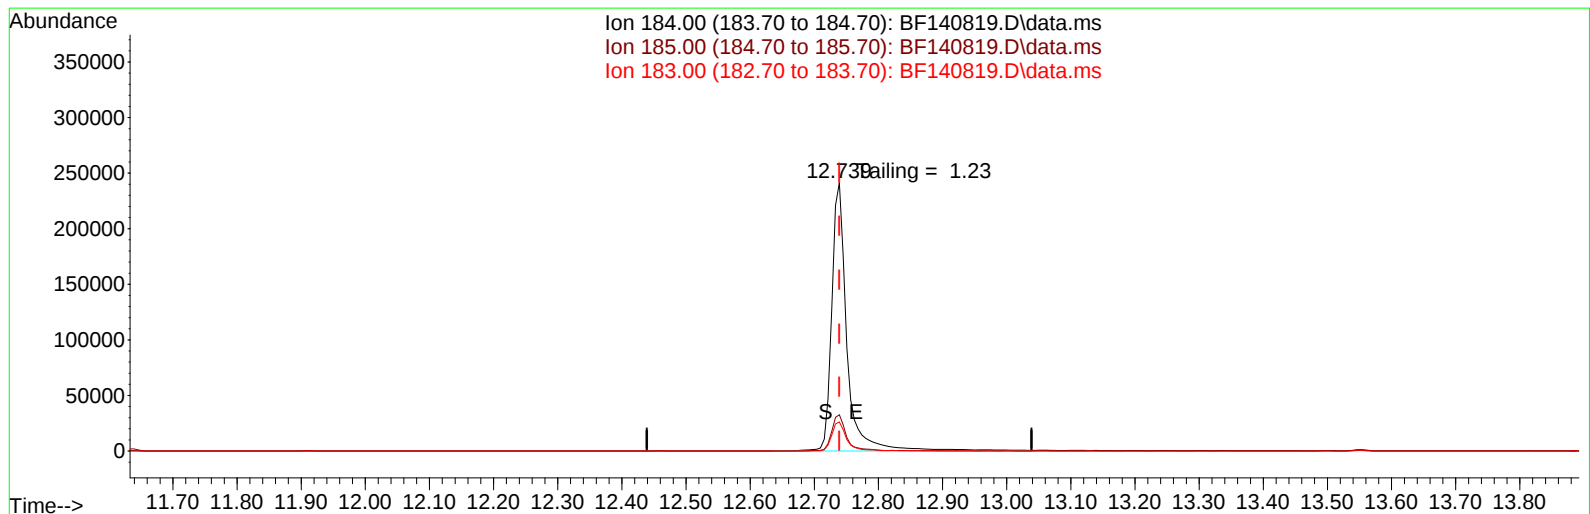

TIC: BF140819.D\data.ms

(77) **Benzidine**

12.739min (+ 0.000) 12781.12 ng

response **393900**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	13.58
183.00	11.00	10.89
0.00	0.00	0.00