


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121218\
 Data File : BF111321.D
 Acq On : 12 Dec 2018 15:05
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF121218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 12 13:16:52 2018

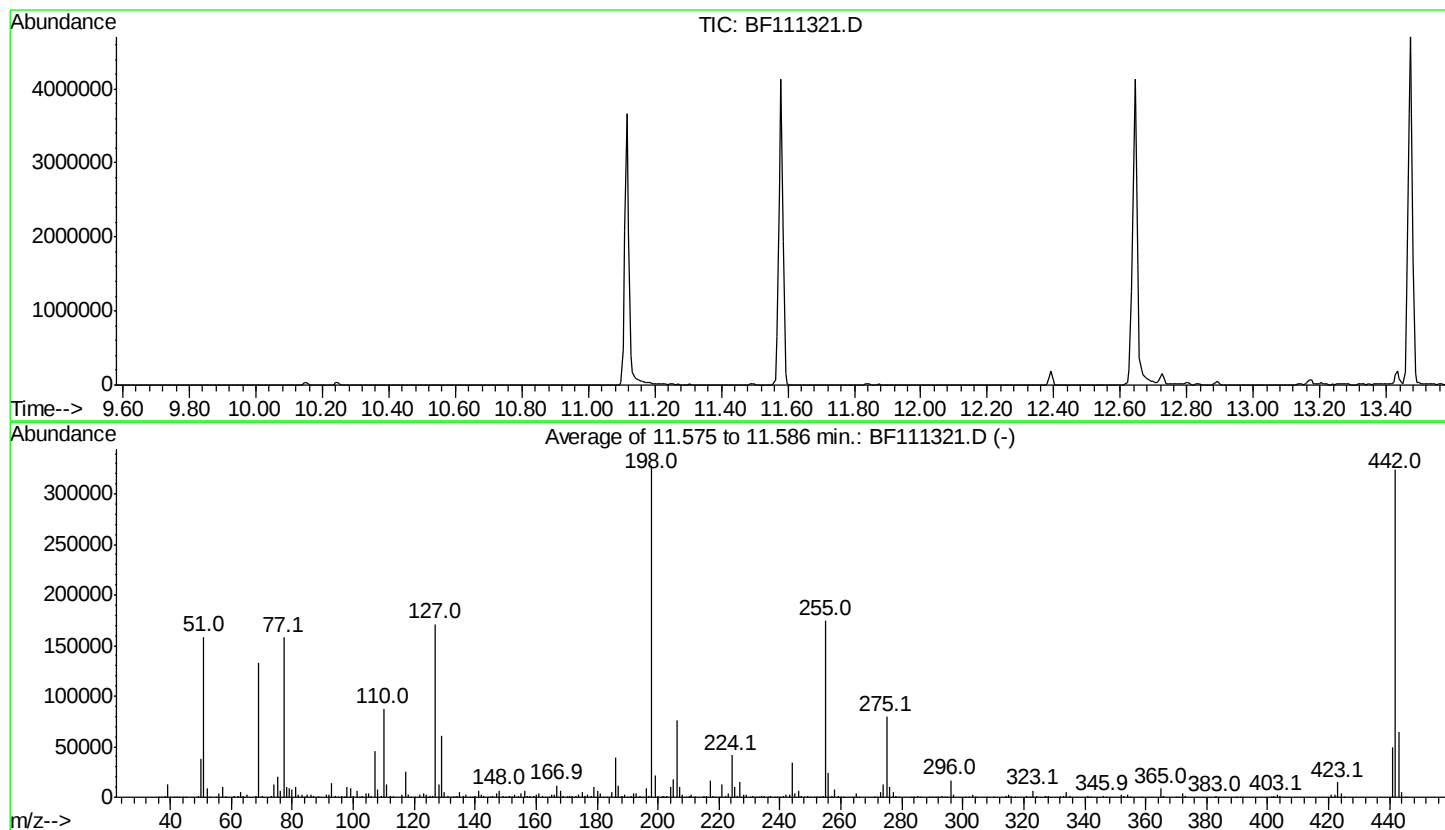

AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.4	158829	PASS
68	69	0.00	2	1.4	1810	PASS
69	198	0.00	100	40.6	133309	PASS
70	69	0.00	2	0.6	835	PASS
127	198	10	80	52.2	171162	PASS
197	198	0.00	2	0.5	1678	PASS
198	198	100	100	100.0	328000	PASS
199	198	5	9	6.7	22137	PASS
275	198	10	60	24.3	79749	PASS
365	198	1	100	2.6	8483	PASS
441	198	0.01	100	15.1	49669	PASS
442	198	50	100	99.0	324693	PASS
443	442	15	24	19.8	64133	PASS