


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121218\
 Data File : BF111348.D
 Acq On : 13 Dec 2018 3:57
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF121218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 12 13:16:52 2018

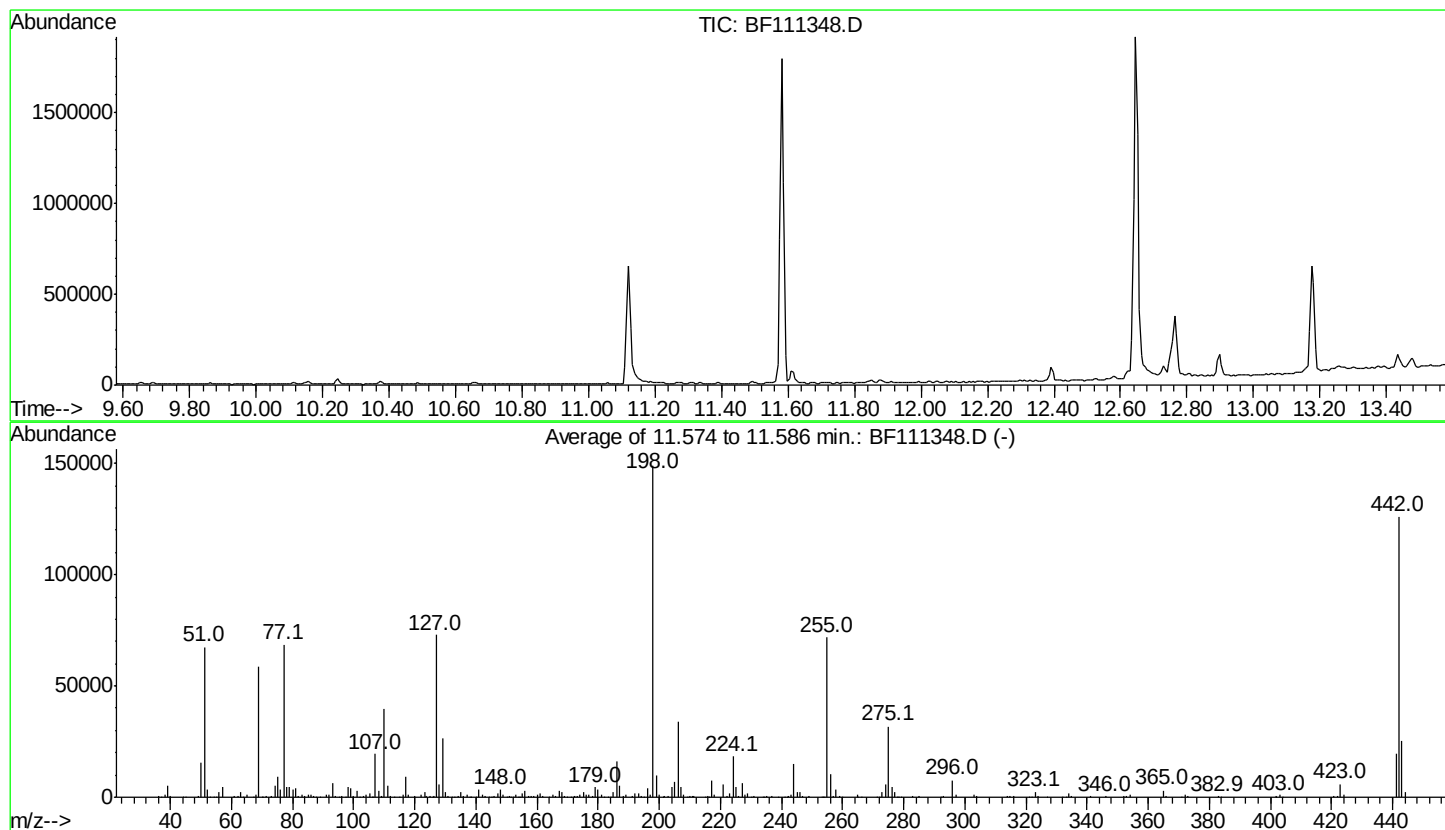

AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.3	67526	PASS
68	69	0.00	2	1.7	1015	PASS
69	198	0.00	100	39.2	58403	PASS
70	69	0.00	2	0.4	214	PASS
127	198	10	80	48.9	72845	PASS
197	198	0.00	2	0.6	895	PASS
198	198	100	100	100.0	148968	PASS
199	198	5	9	6.6	9855	PASS
275	198	10	60	21.3	31782	PASS
365	198	1	100	2.1	3144	PASS
441	198	0.01	100	13.1	19535	PASS
442	198	50	100	84.6	125997	PASS
443	442	15	24	20.1	25299	PASS