
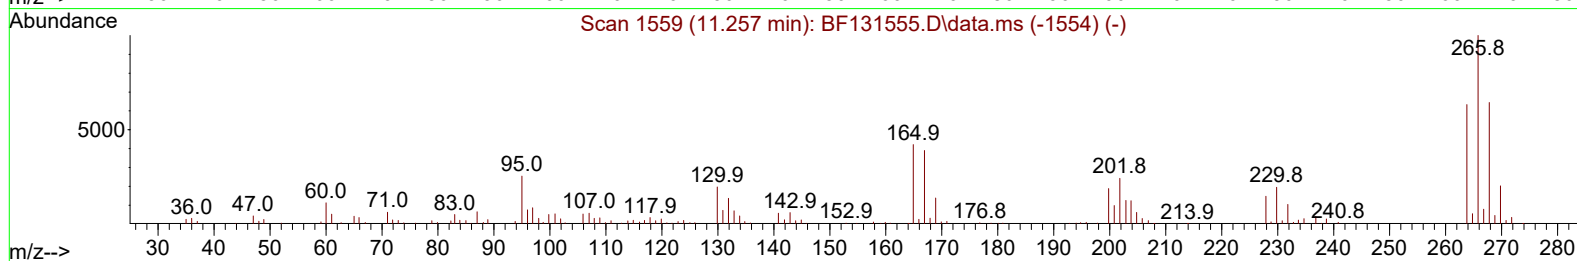
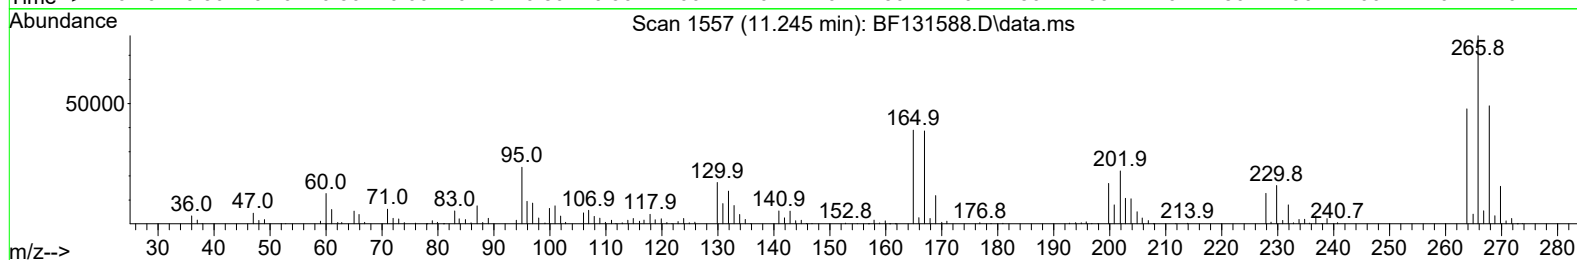


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121222\
 Data File : BF131588.D
 Acq On : 12 Dec 2022 12:09
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 13 07:56:30 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 13 04:12:13 2022
 Response via : Initial Calibration

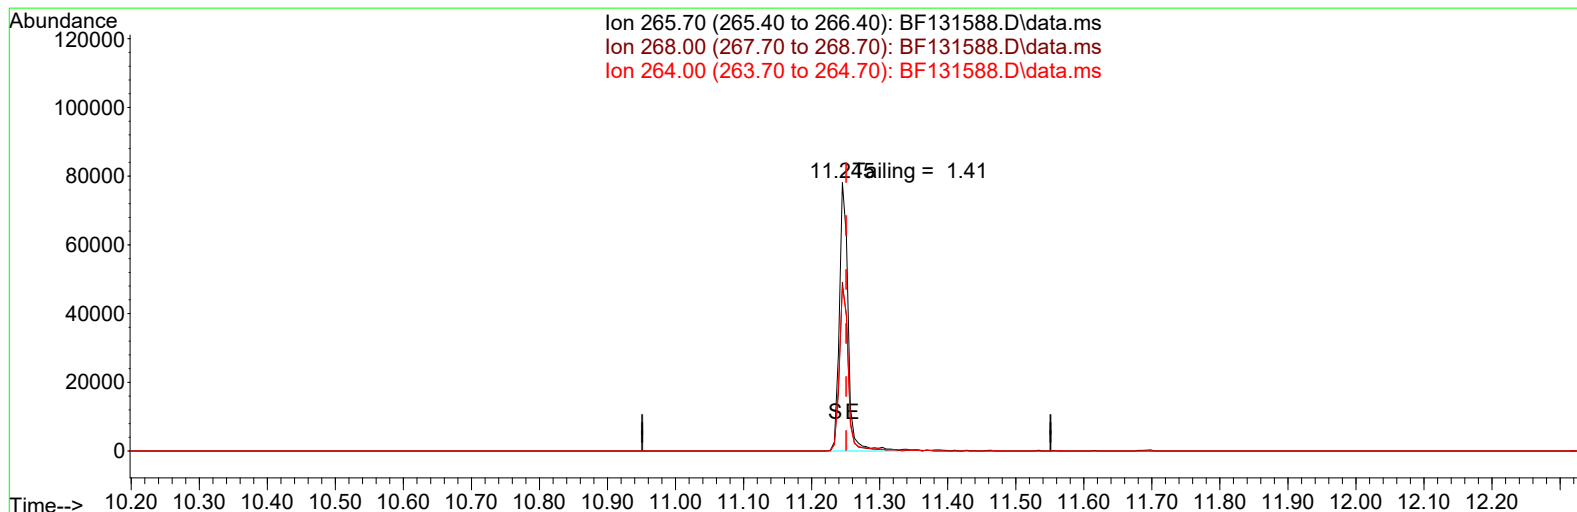

TIC: BF131588.D\data.ms

(70) Pentachlorophenol (C)

11.245min (-0.006) 34030.03 ng

response 69963

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.40	62.82
264.00	63.40	61.16
0.00	0.00	0.00

