
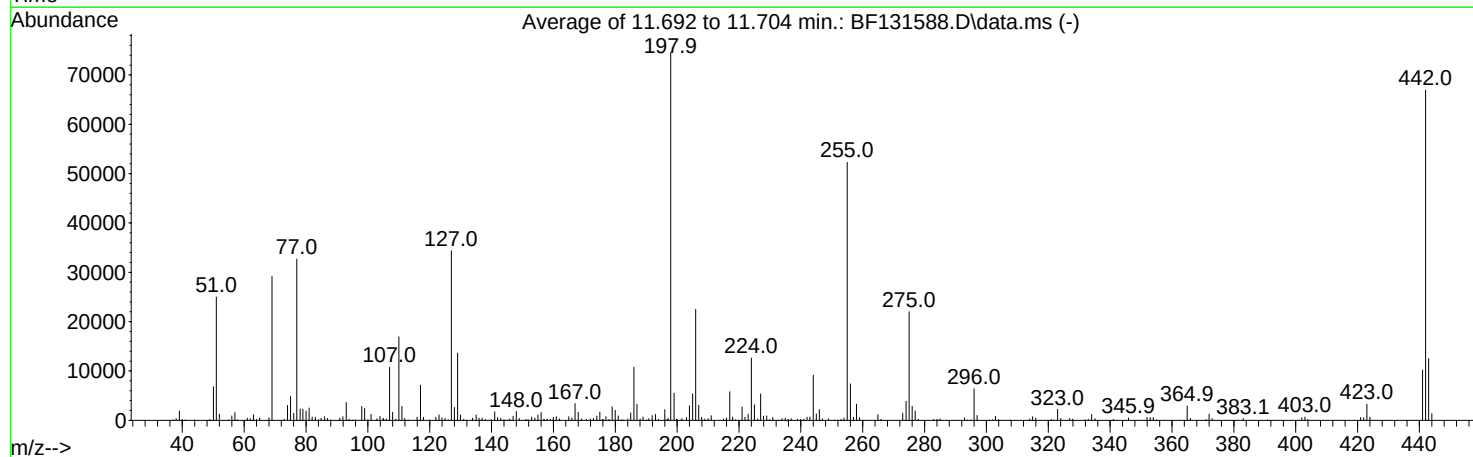


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121222\
 Data File : BF131588.D
 Acq On : 12 Dec 2022 12:09
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 13 04:12:13 2022

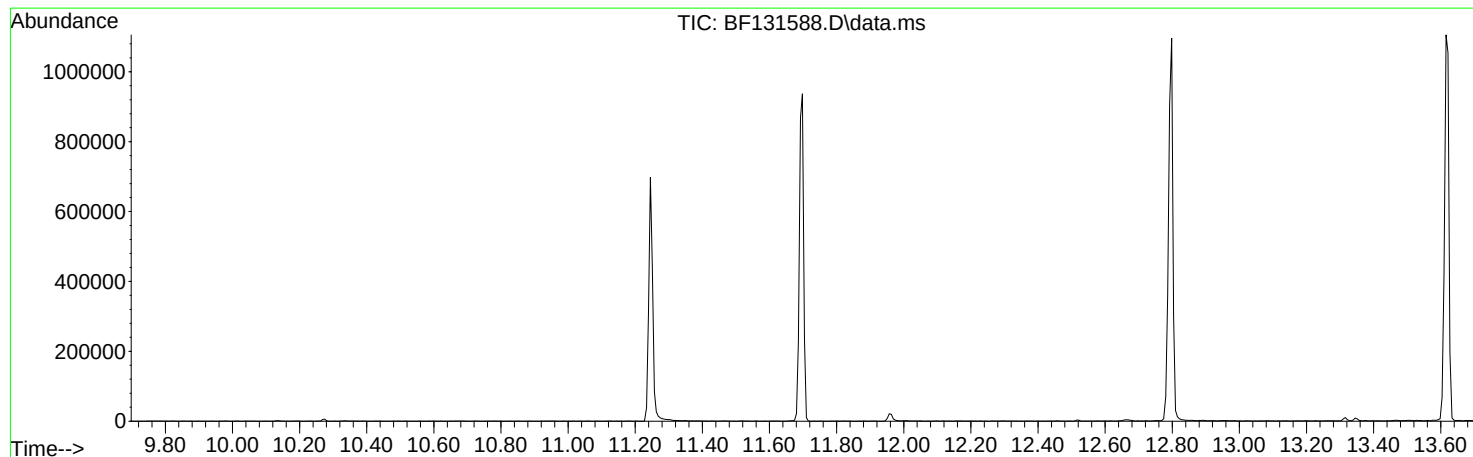




AutoFind: Scans 1633, 1634, 1635; Background Corrected with Scan 1627

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.5	24980	PASS
68	69	0.00	2	1.8	522	PASS
69	198	0.00	100	39.1	29185	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.1	34374	PASS
197	198	0.00	2	0.4	333	PASS
198	198	100	100	100.0	74565	PASS
199	198	5	9	7.4	5490	PASS
275	198	10	60	29.5	22001	PASS
365	198	1	100	3.9	2895	PASS
441	198	0.01	100	13.6	10169	PASS
442	442	50	100	100.0	66941	PASS
443	442	15	24	18.7	12519	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121222\
Data File : BF131588.D
Acq On : 12 Dec 2022 12:09
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 13 07:56:30 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 13 04:12:13 2022
Response via : Initial Calibration

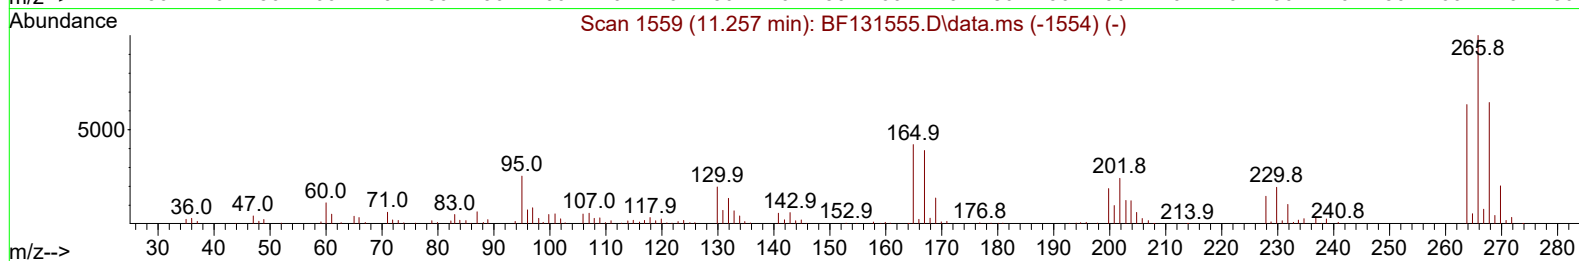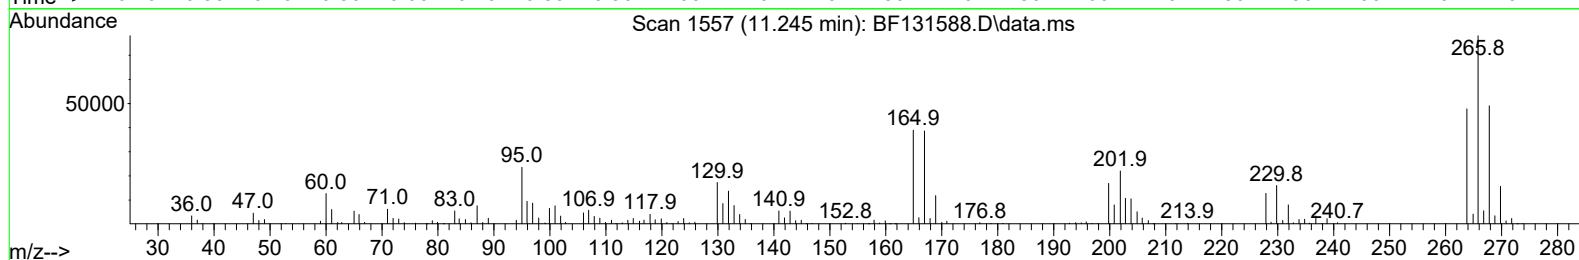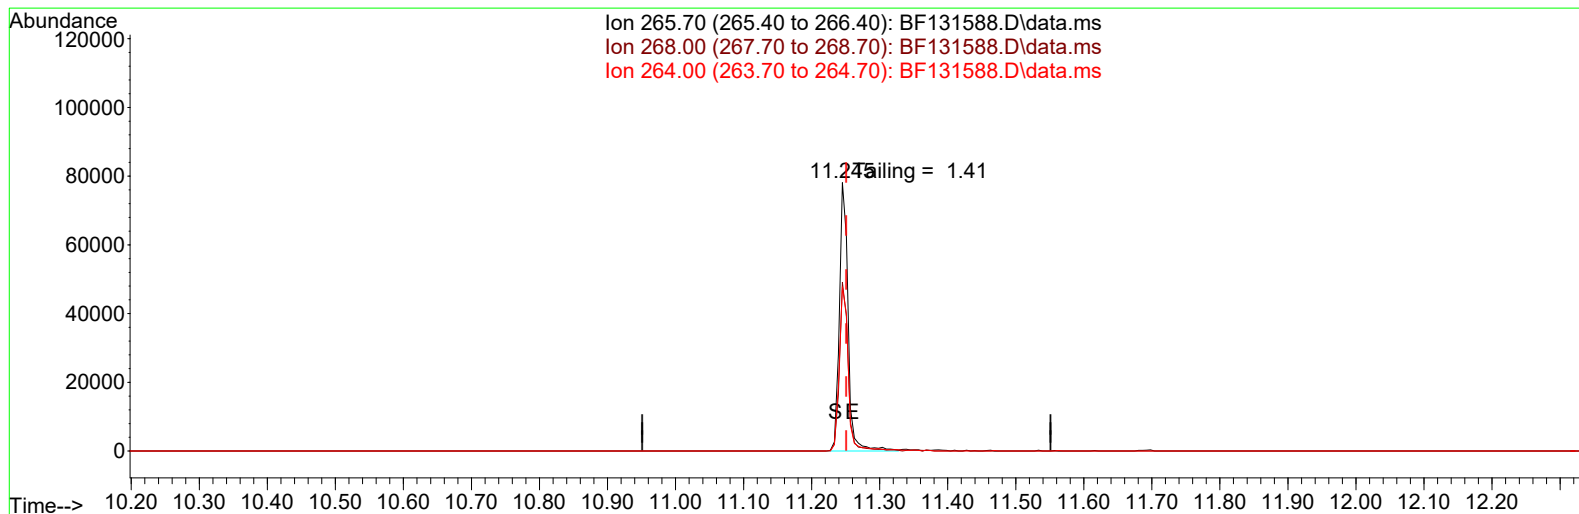

TIC: BF131588.D\data.ms

(70) Pentachlorophenol (C)

11.245min (-0.006) 34030.03 ng




response 69963

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.40	62.82
264.00	63.40	61.16
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121222\  
Data File : BF131588.D  
Acq On    : 12 Dec 2022  12:09  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 13 07:56:30 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 13 04:12:13 2022
Response via : Initial Calibration

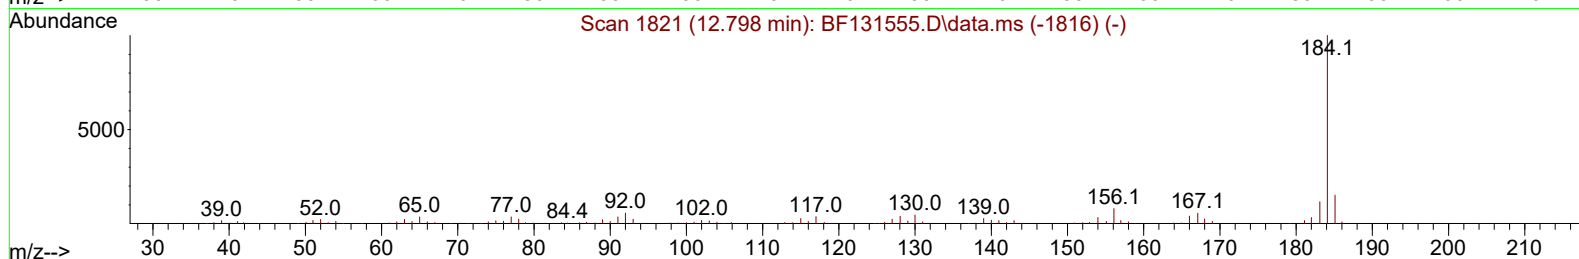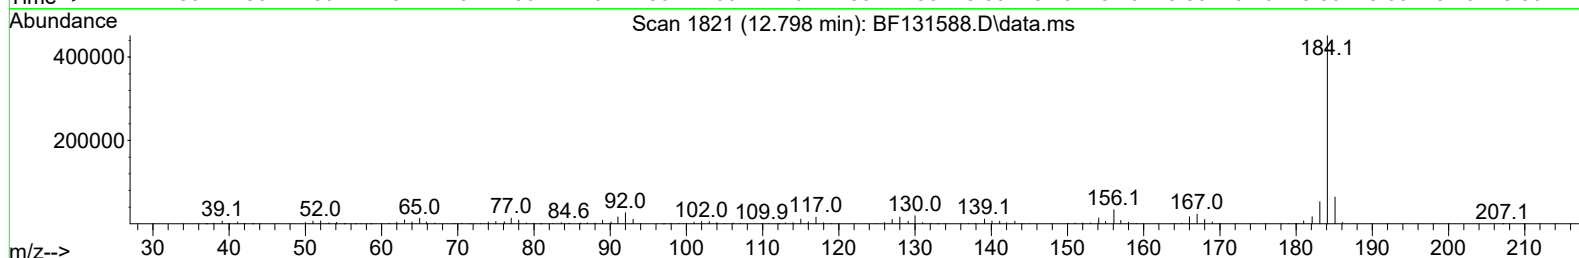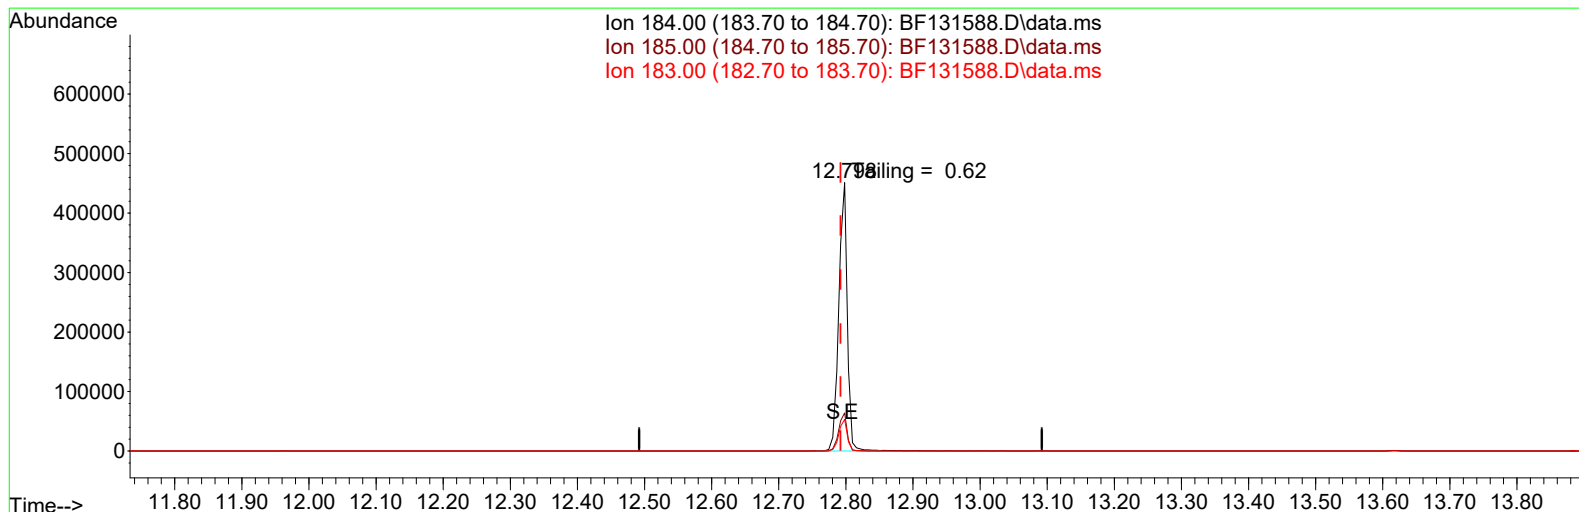

TIC: BF131588.D\data.ms

(77) Benzidine

12.798min (+ 0.006) 0.00 ng

response **400549**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.21
183.00	11.60	11.78
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/12/2022	BNA_F	<u>BF131588.D</u>
Compound Name	Response	Retention Time
DDT	198016	13.622
DDD	3685	13.316
DDE	194	12.975
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3879	201895	1.92

Instrument :
BNA_F
ClientSampleId :
DFTPP