
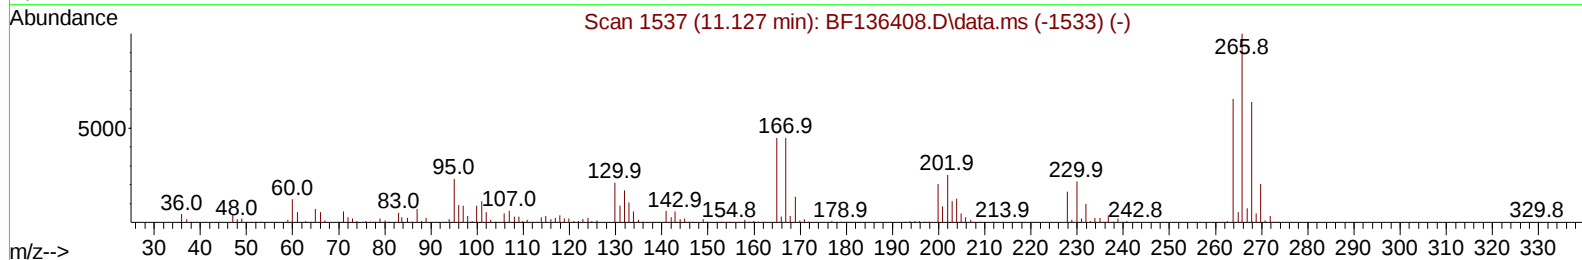
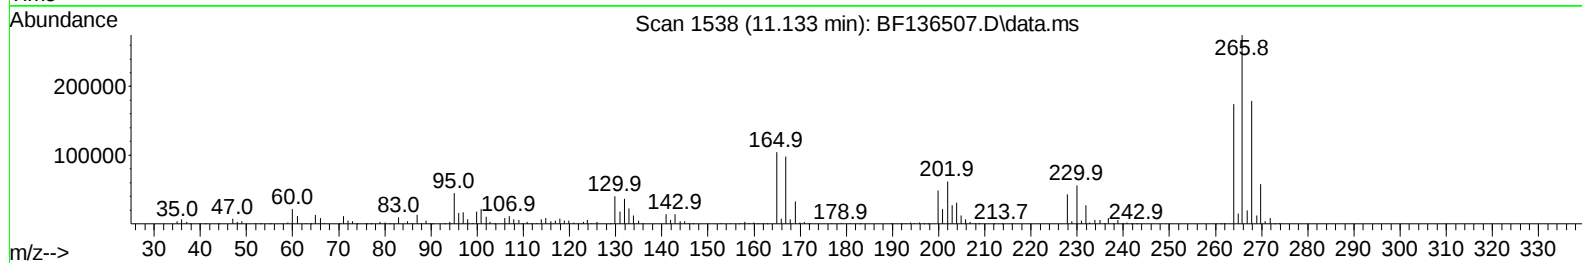


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121223\
Data File : BF136507.D
Acq On : 12 Dec 2023 10:21
Operator : CG\JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 13 00:17:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 06 09:40:27 2023
Response via : Initial Calibration

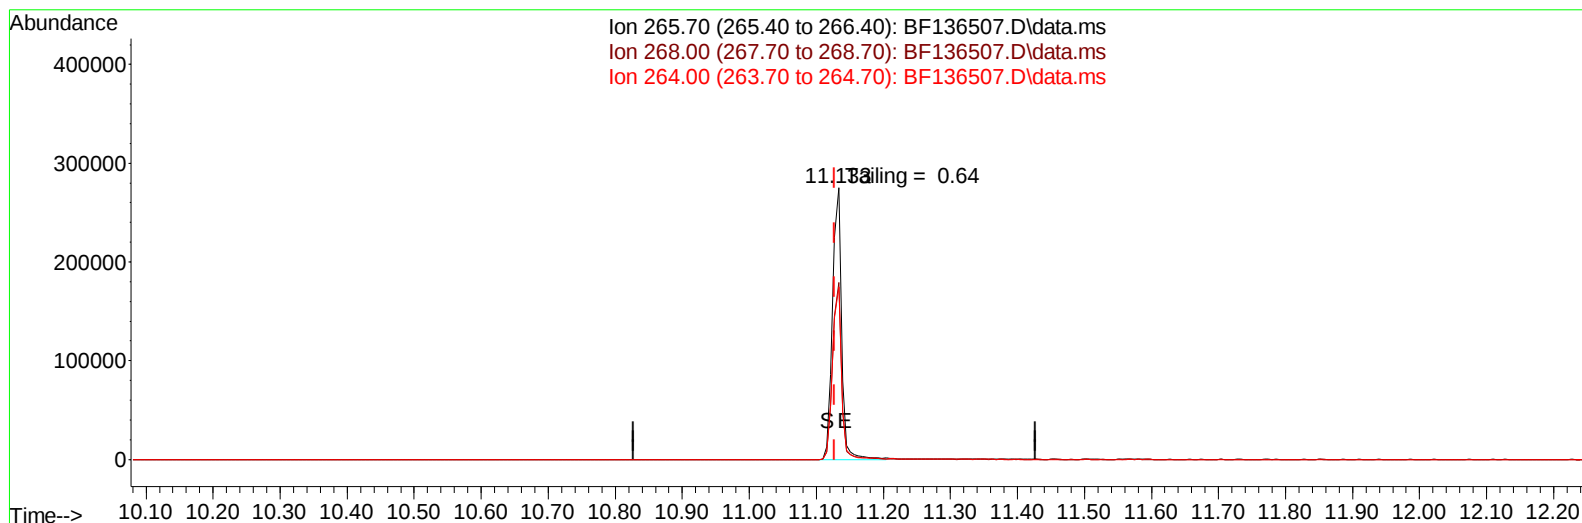

TIC: BF136507.D\data.ms

(70) Pentachlorophenol (C)




11.133min (+ 0.006) 17599.80 ng

response 256276

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	65.20
264.00	65.30	63.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121223\
Data File : BF136507.D
Acq On : 12 Dec 2023 10:21
Operator : CG\JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 13 00:17:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 06 09:40:27 2023
Response via : Initial Calibration

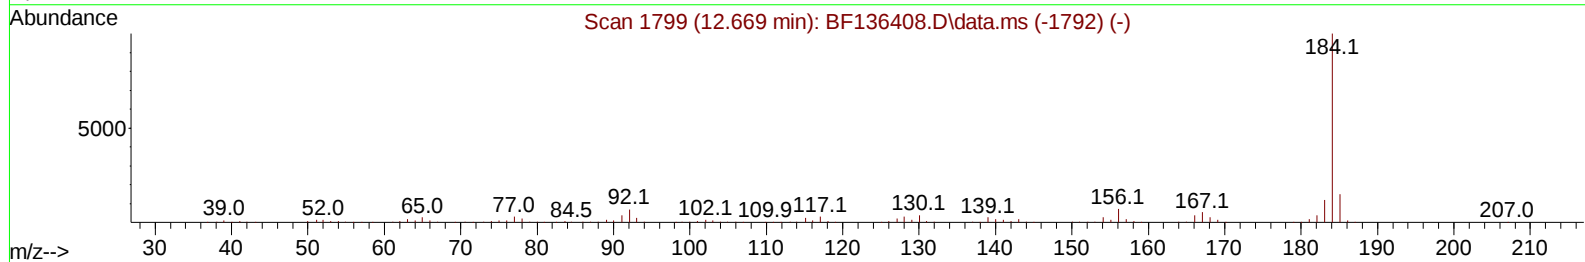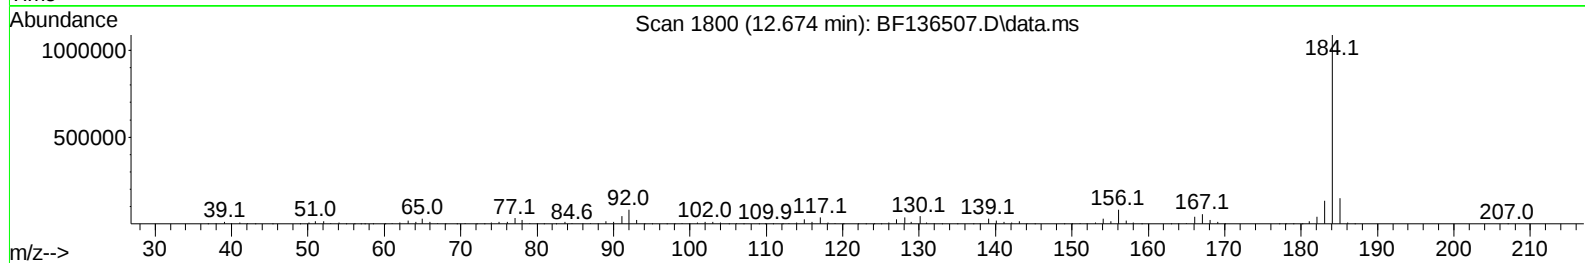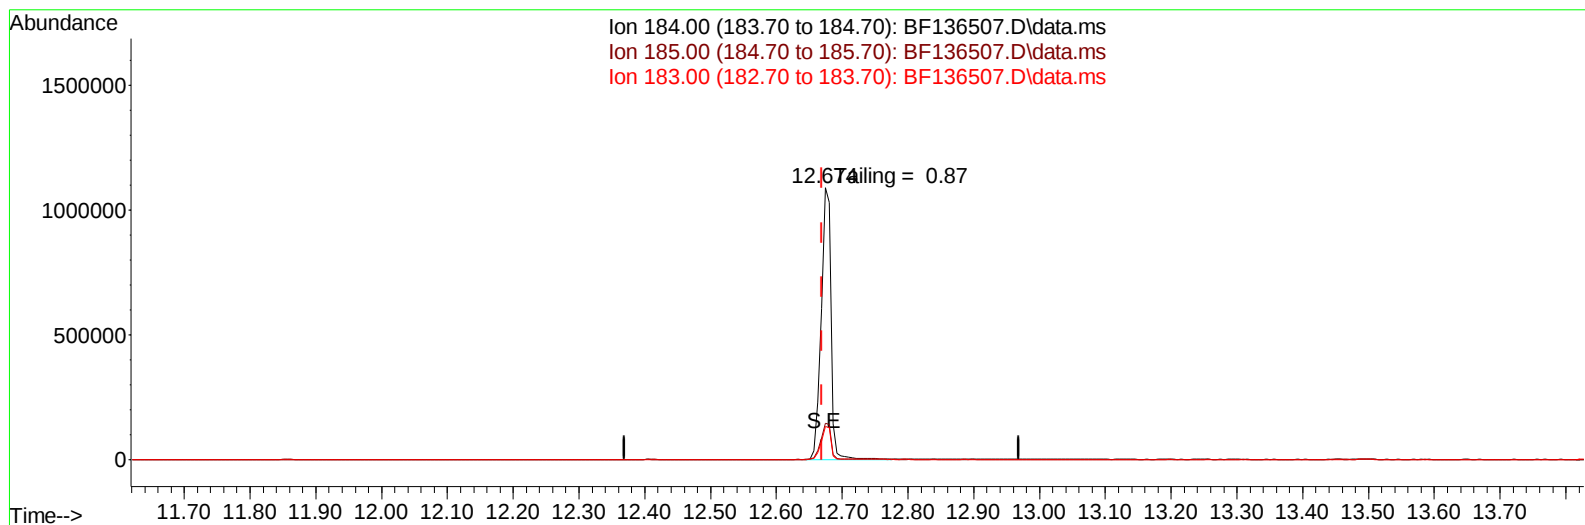

TIC: BF136507.D\data.ms

(77) Benzidine

12.674min (+ 0.005) 1430.24 ng

response 1144944

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	13.45
183.00	11.70	12.12
0.00	0.00	0.00