


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121223\
Data File : BF136507.D
Acq On : 12 Dec 2023 10:21
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Dec 06 09:40:27 2023

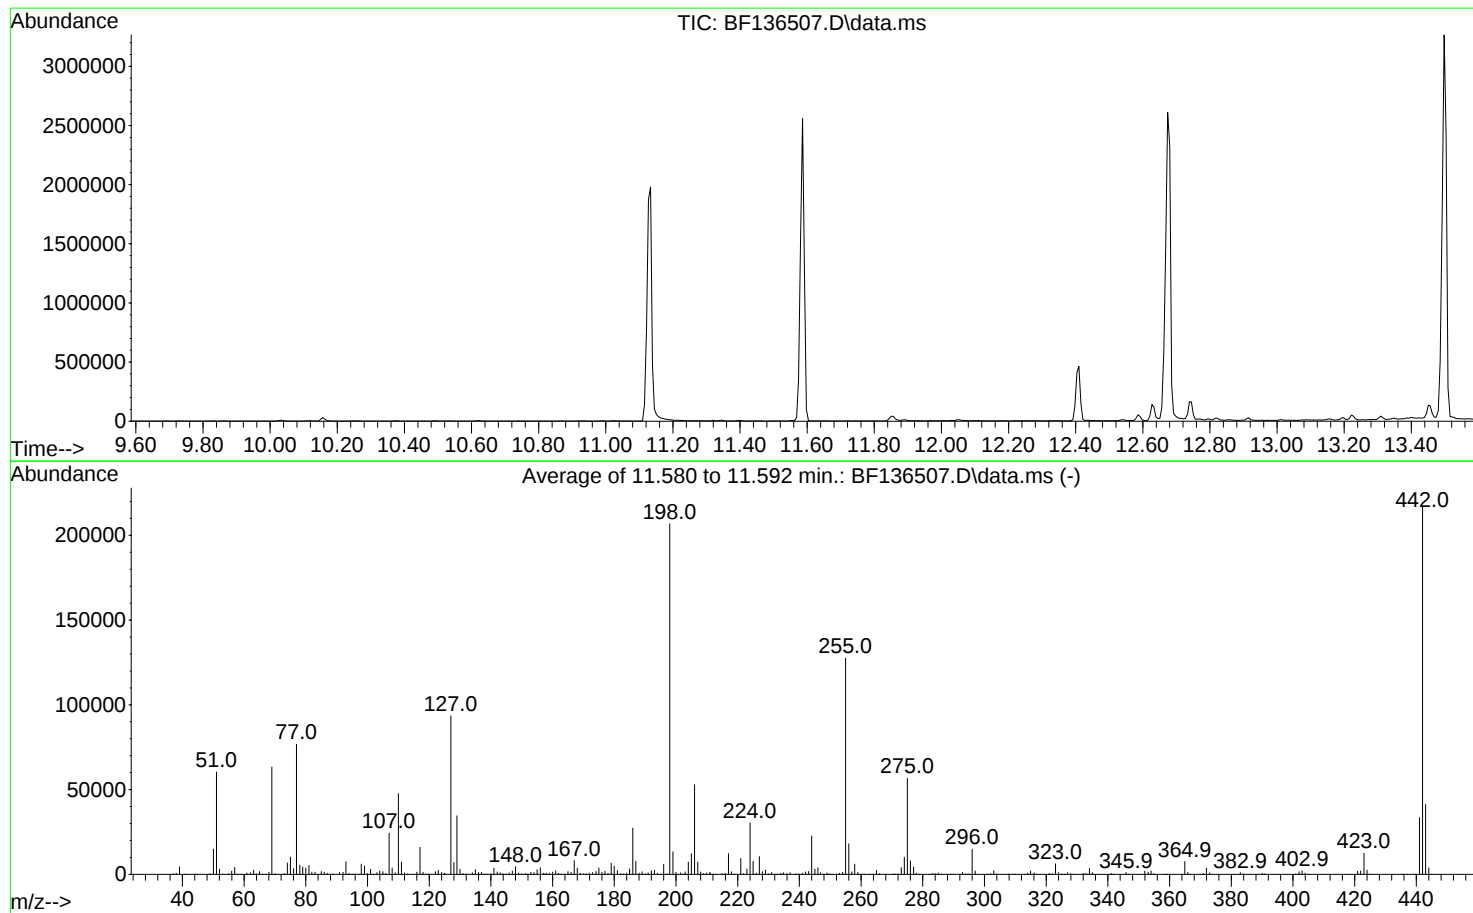




AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.2	60400	PASS
68	69	0.00	2	1.9	1203	PASS
69	198	0.00	100	30.6	63371	PASS
70	69	0.00	2	0.4	280	PASS
127	198	10	80	45.2	93419	PASS
197	198	0.00	2	0.2	424	PASS
198	198	100	100	100.0	206789	PASS
199	198	5	9	6.4	13321	PASS
275	198	10	60	27.4	56643	PASS
365	198	1	100	3.7	7602	PASS
441	198	0.01	100	16.2	33408	PASS
442	442	50	100	100.0	216997	PASS
443	442	15	24	19.0	41131	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121223\
Data File : BF136507.D
Acq On : 12 Dec 2023 10:21
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 13 00:17:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 06 09:40:27 2023
Response via : Initial Calibration

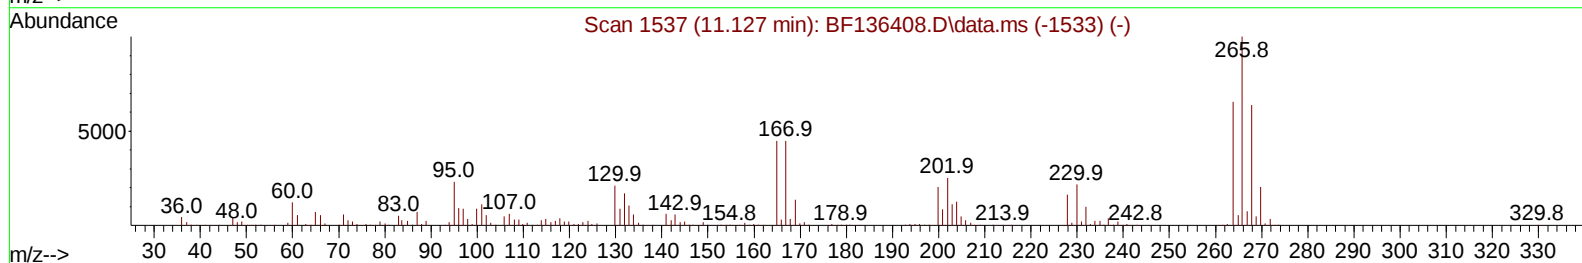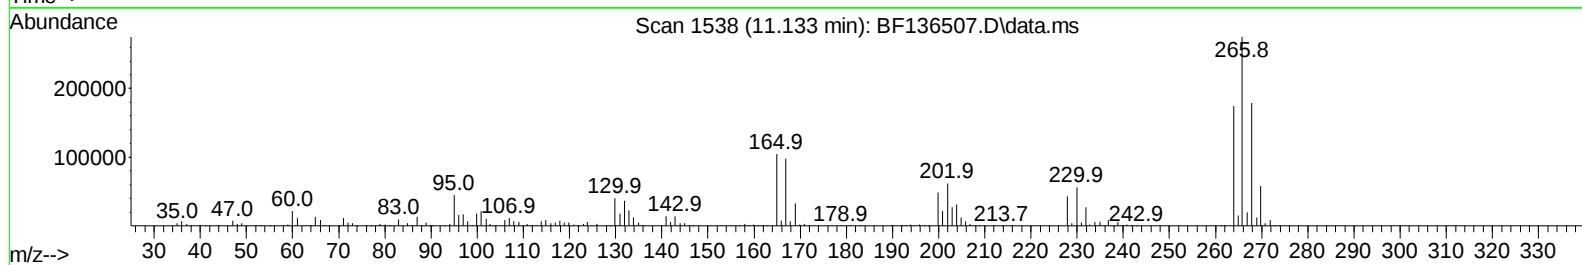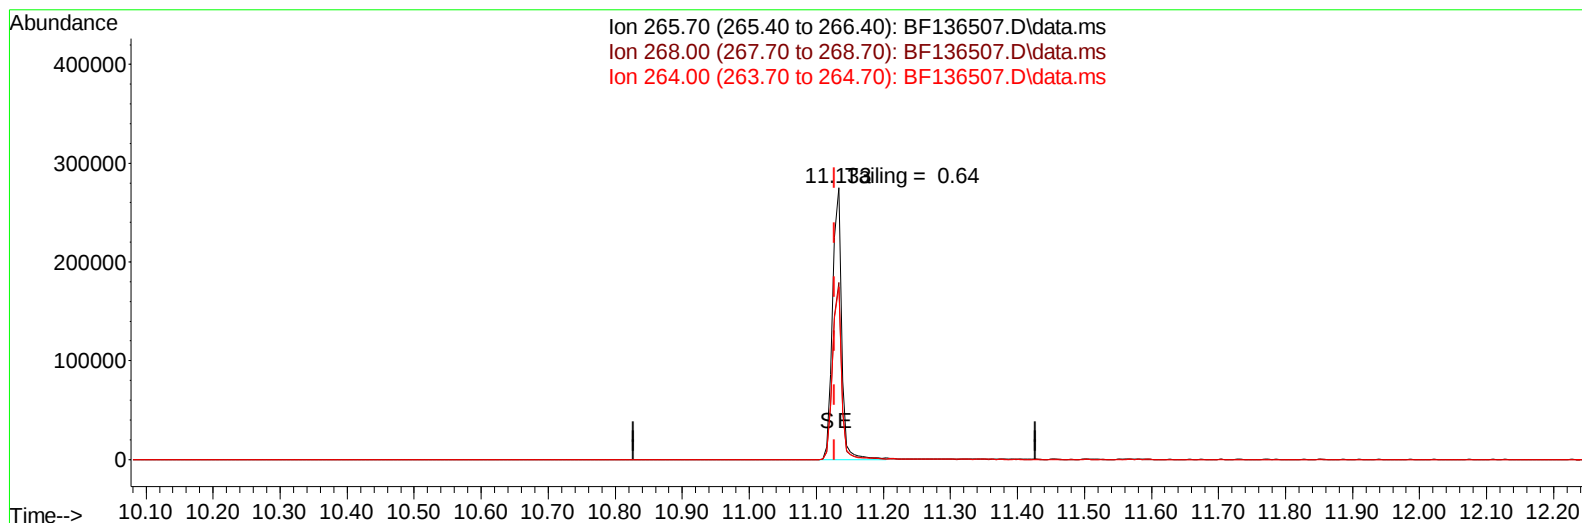

TIC: BF136507.D\data.ms

(70) Pentachlorophenol (C)

11.133min (+ 0.006) 17599.80 ng




response 256276

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	65.20
264.00	65.30	63.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121223\
Data File : BF136507.D
Acq On : 12 Dec 2023 10:21
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 13 00:17:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 06 09:40:27 2023
Response via : Initial Calibration

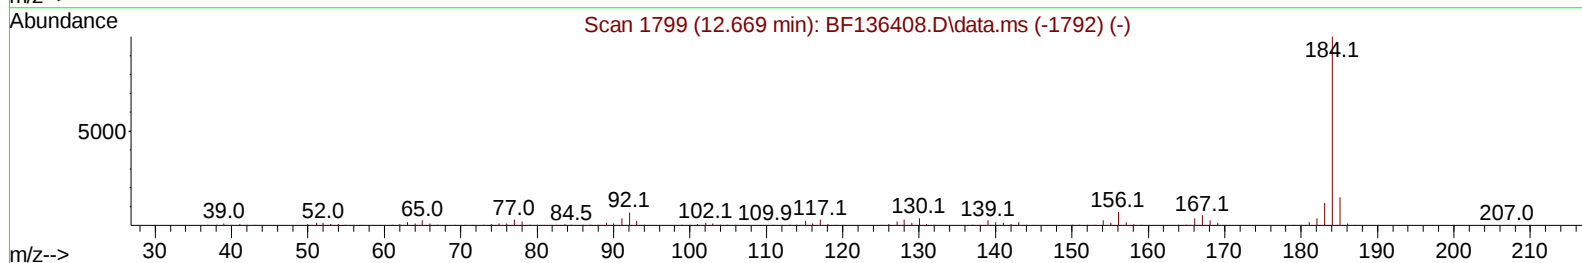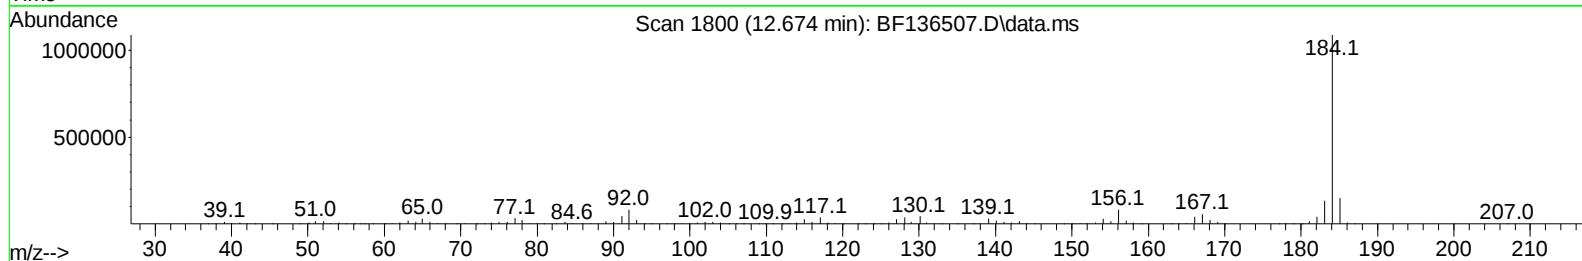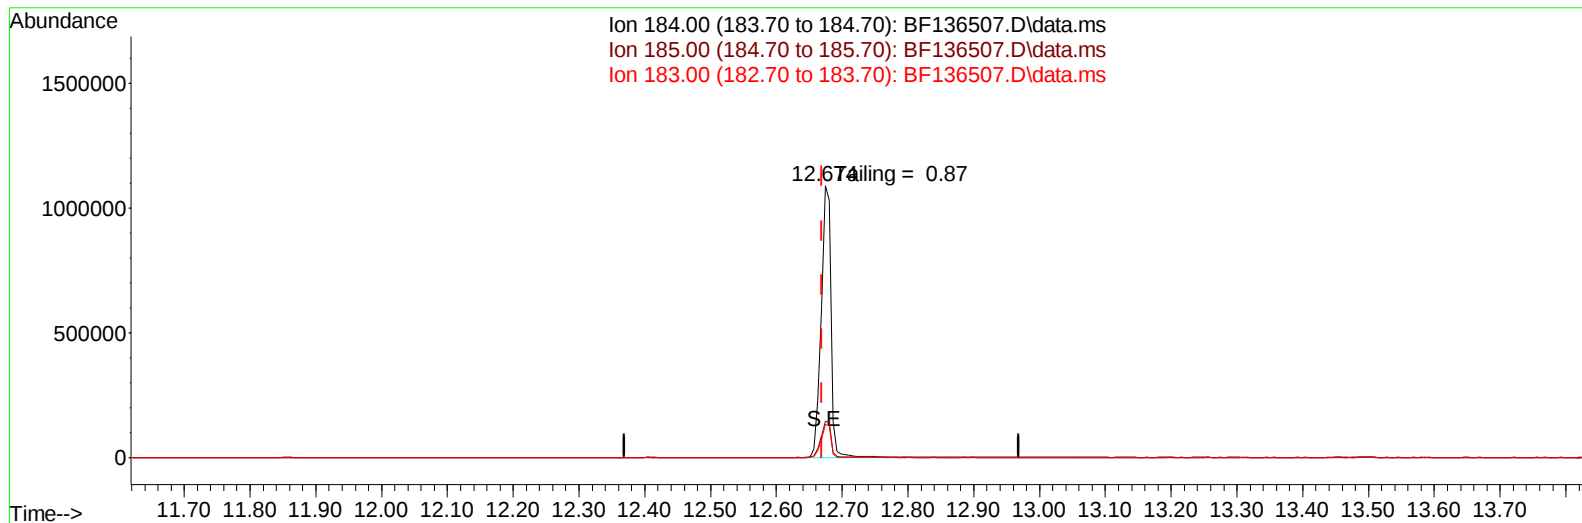

TIC: BF136507.D\data.ms

(77) Benzidine

12.674min (+ 0.005) 1430.24 ng

response 1144944

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	13.45
183.00	11.70	12.12
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/12/2023	BNA_F	<u>BF136507.D</u>
Compound Name	Response	Retention Time
DDT	613953	13.498
DDD	10008	13.227
DDE	675	12.857
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10683	624636	1.71

Instrument :
BNA_F
ClientSampleId :
DFTPP