
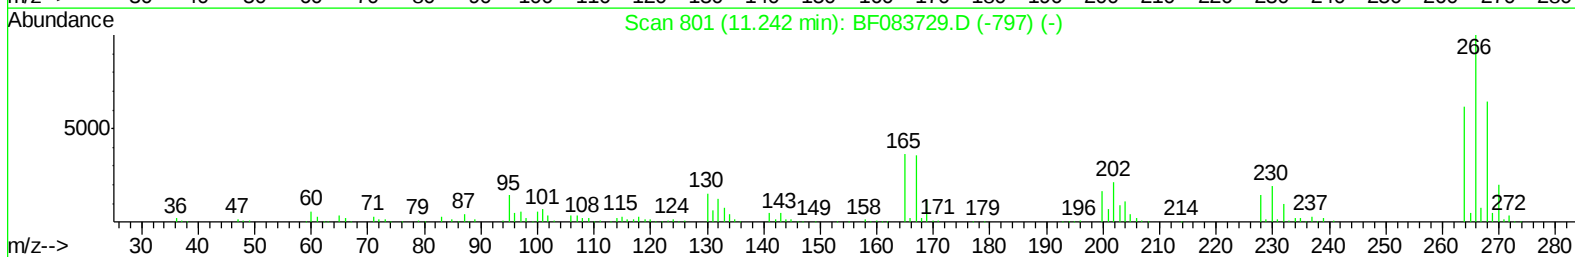
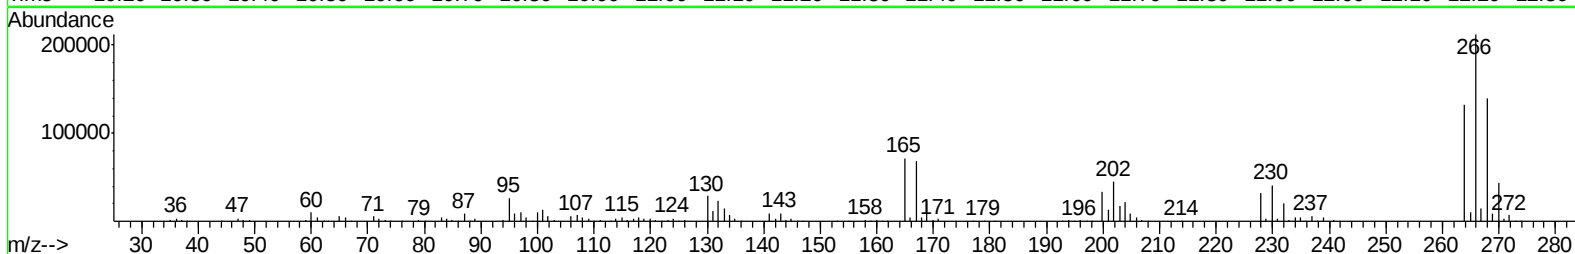


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF121315\
Data File : BF083725.D
Acq On : 13 Dec 2015 12:28
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 14 07:33:04 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 14 01:30:12 2015
Response via : Initial Calibration

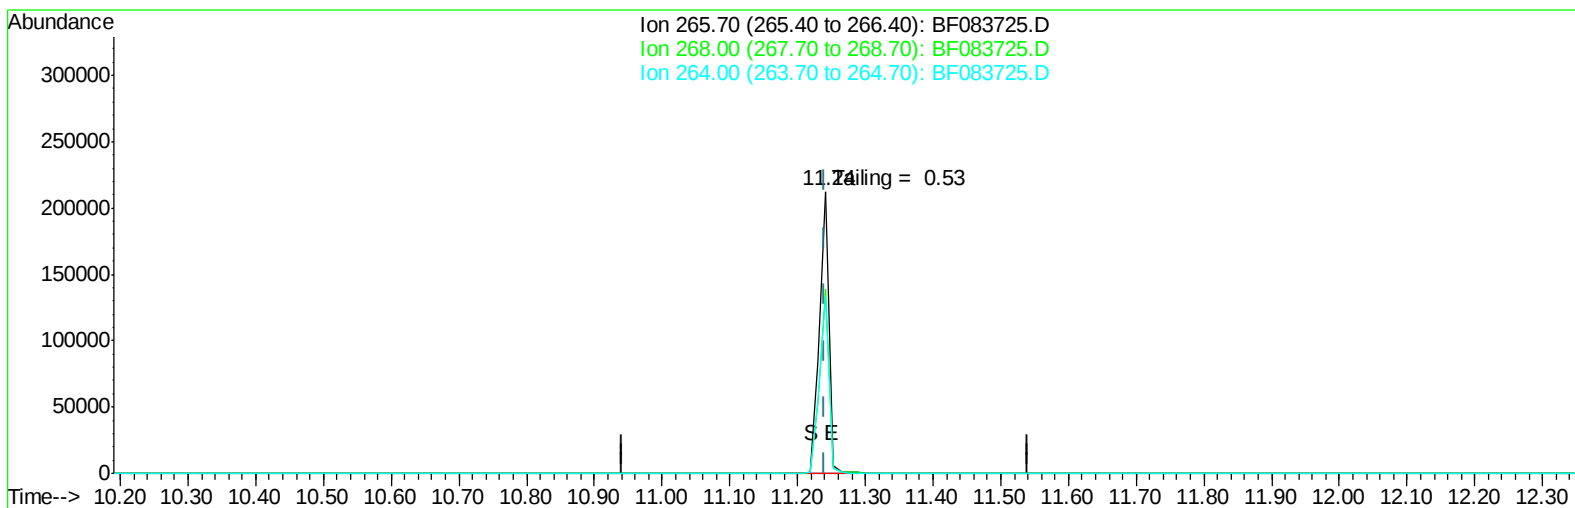

TIC: BF083725.D

(69) Pentachlorophenol (C)




11.242min (+0.001) 0.00ng

response 211477

Ion	Exp%	Act%
265.70	100	100
268.00	62.70	65.63
264.00	64.30	62.53
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF121315\
Data File : BF083725.D
Acq On : 13 Dec 2015 12:28
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 14 07:33:04 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 14 01:30:12 2015
Response via : Initial Calibration

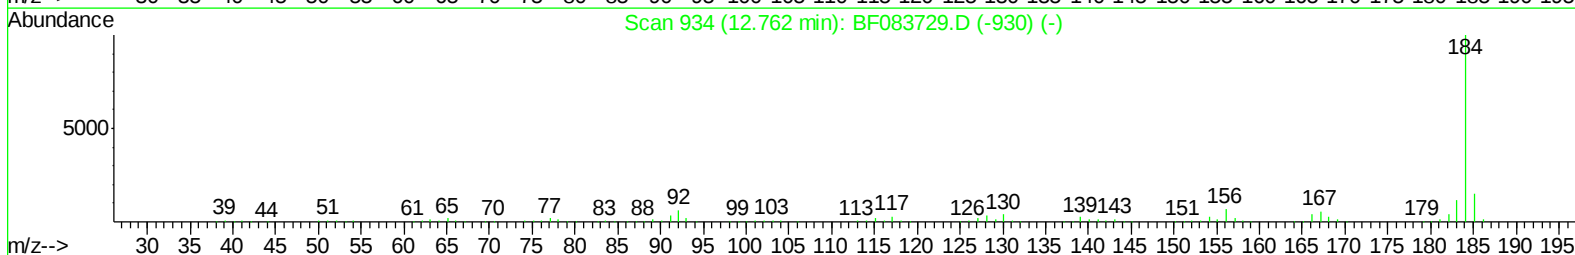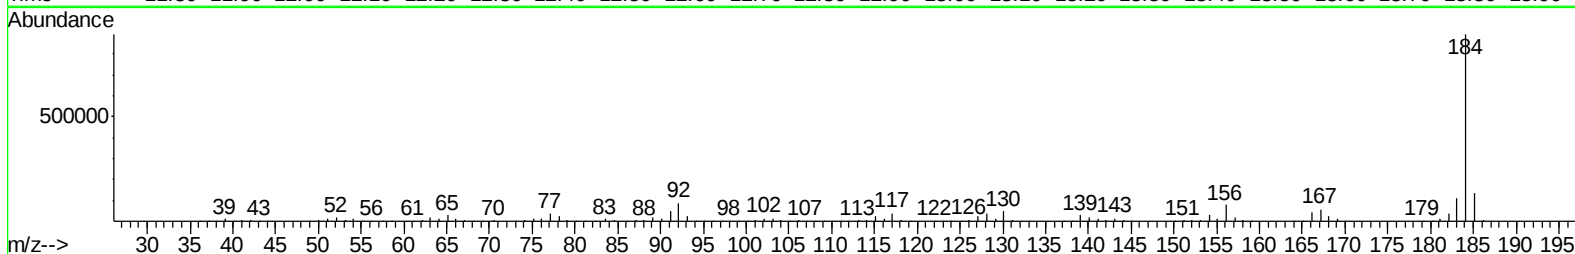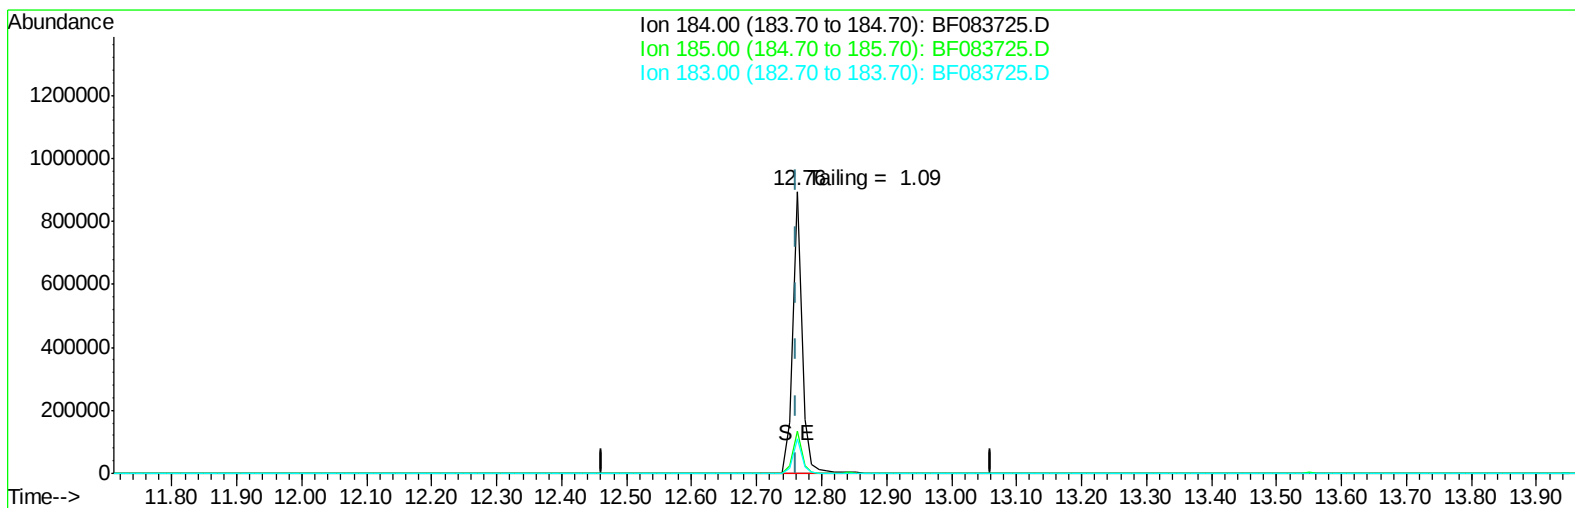

TIC: BF083725.D

(76) Benzidine

12.762min (+0.000) 109651.90ng

response 892148

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	14.92
183.00	11.20	12.49
0.00	0.00	0.00