
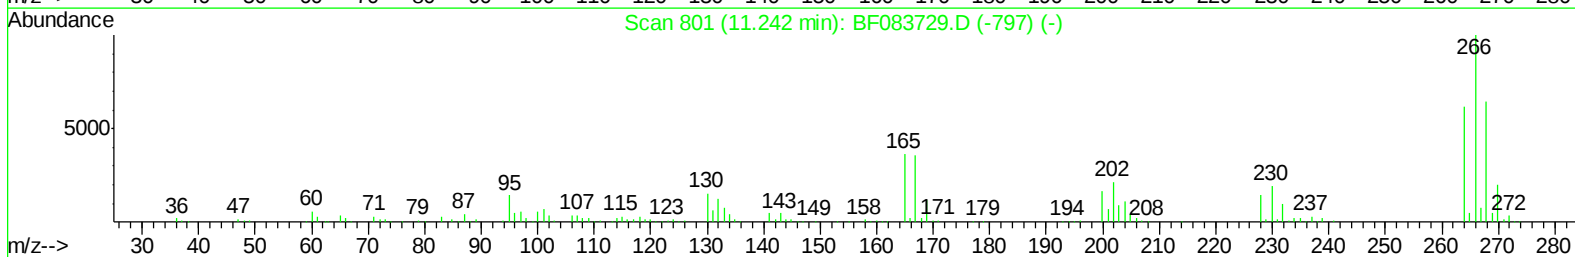
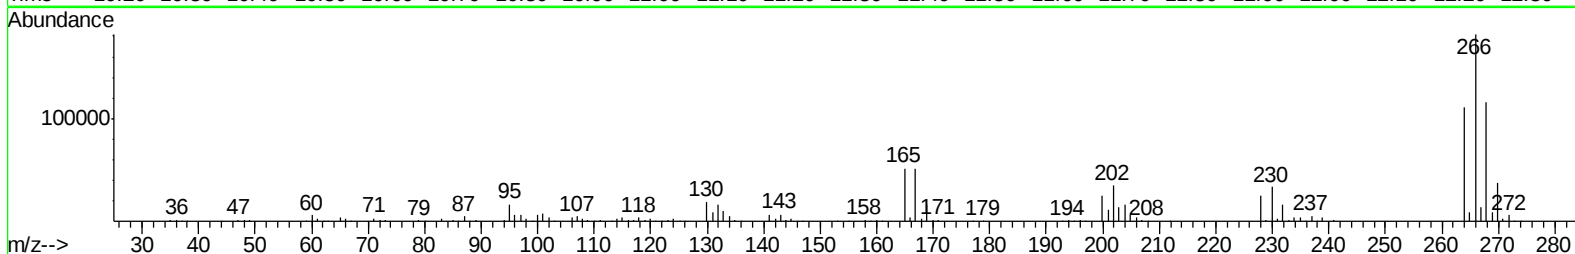


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF121315\
Data File : BF083734.D
Acq On : 13 Dec 2015 17:33
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 14 07:34:15 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 14 01:30:12 2015
Response via : Initial Calibration

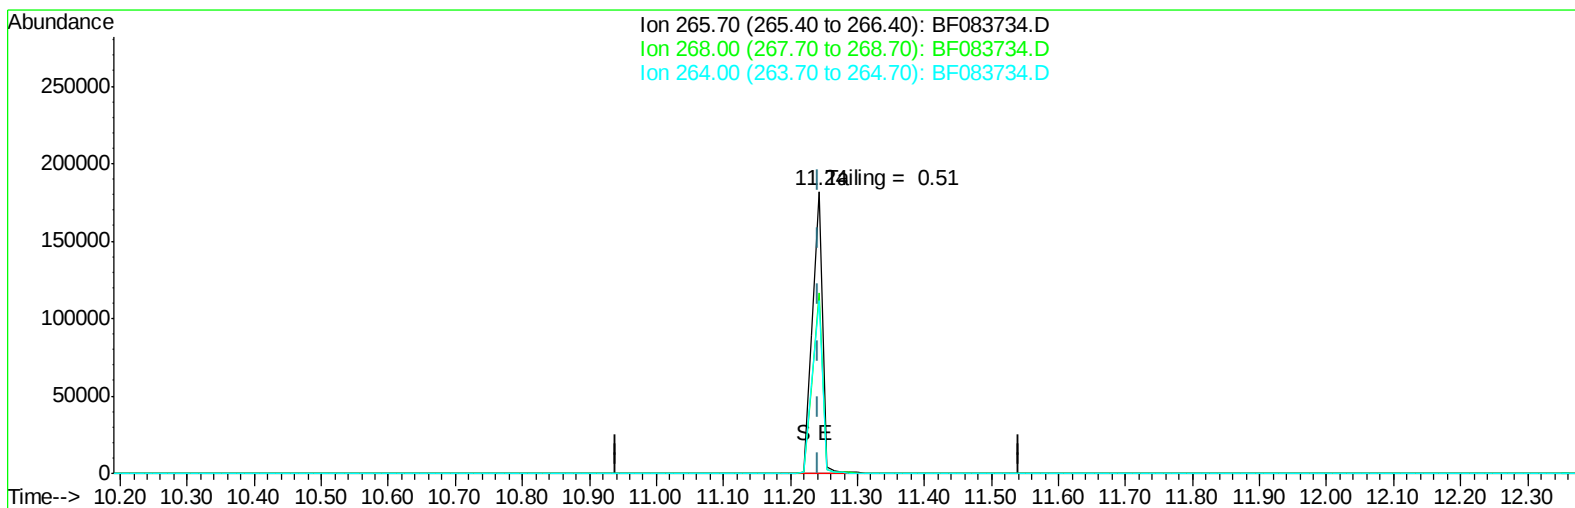

TIC: BF083734.D

(69) Pentachlorophenol (C)




11.242min (+0.001) 0.00ng

response 193066

Ion	Exp%	Act%
265.70	100	100
268.00	62.70	63.93
264.00	64.30	61.37
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF121315\
 Data File : BF083734.D
 Acq On : 13 Dec 2015 17:33
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 14 07:34:15 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121315.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 14 01:30:12 2015
 Response via : Initial Calibration

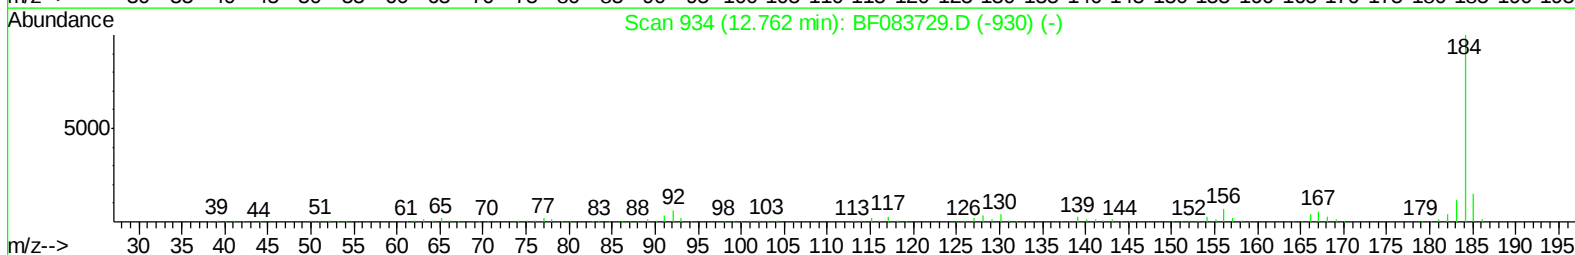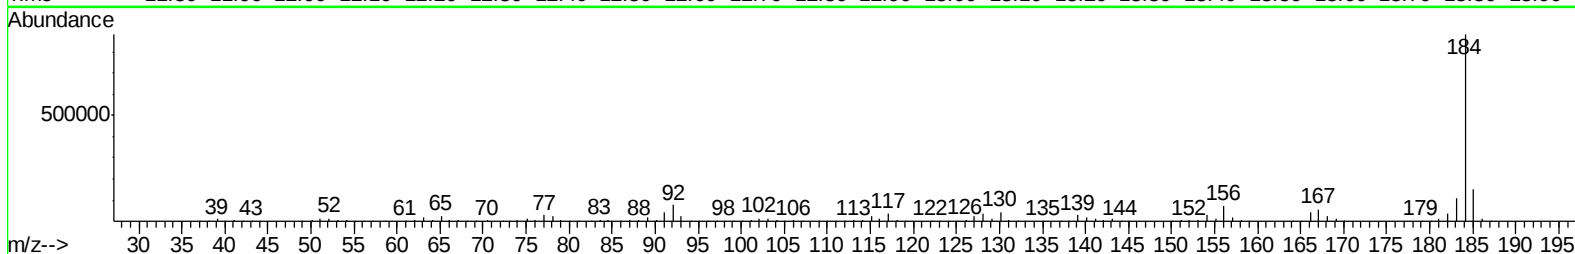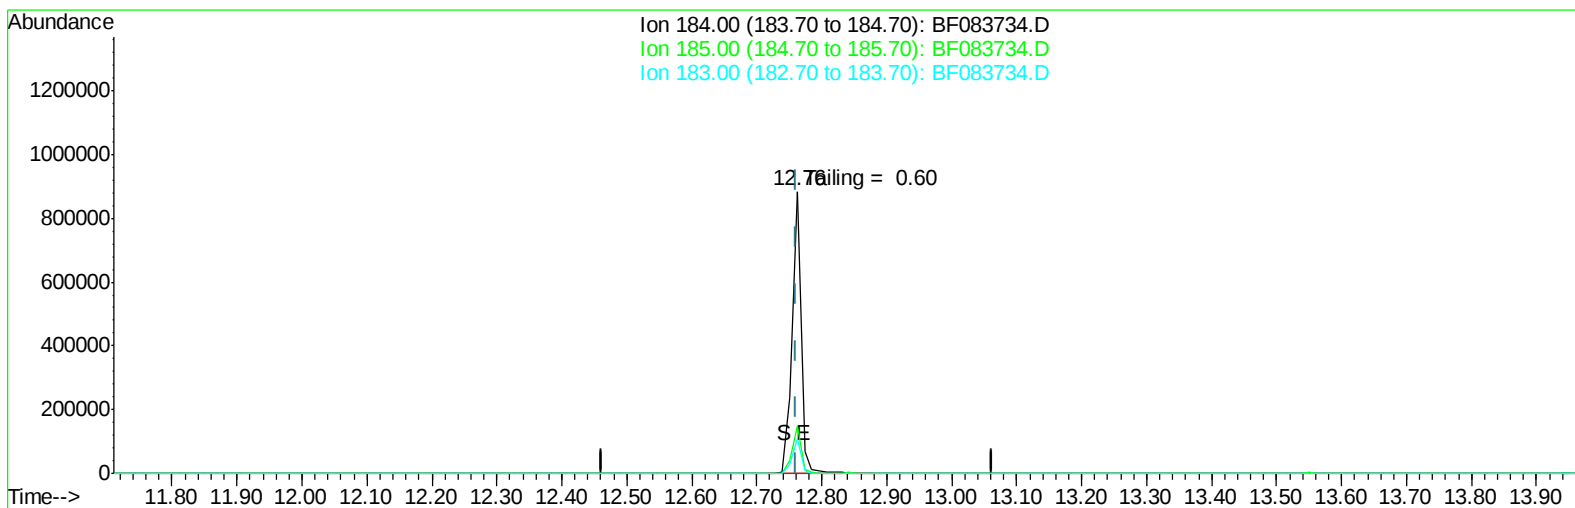

TIC: BF083734.D

(76) Benzidine

12.762min (0.000) 0.00ng

response 844806

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	16.84
183.00	11.20	12.44
0.00	0.00	0.00