
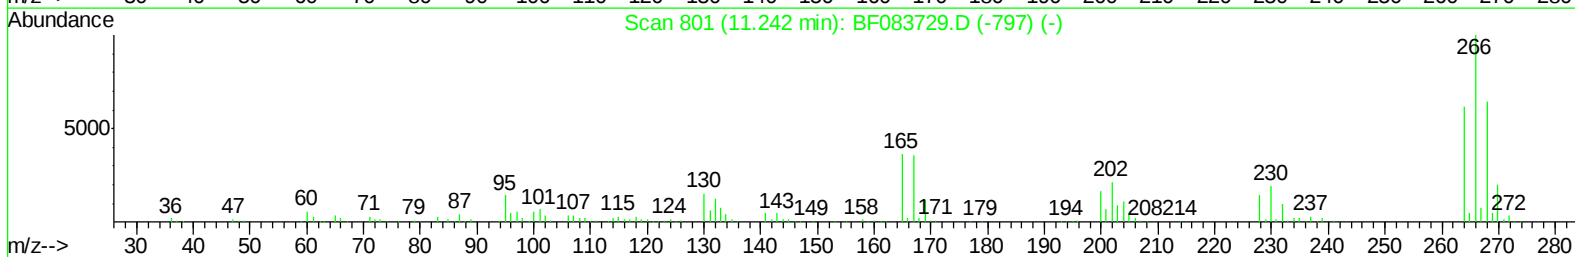
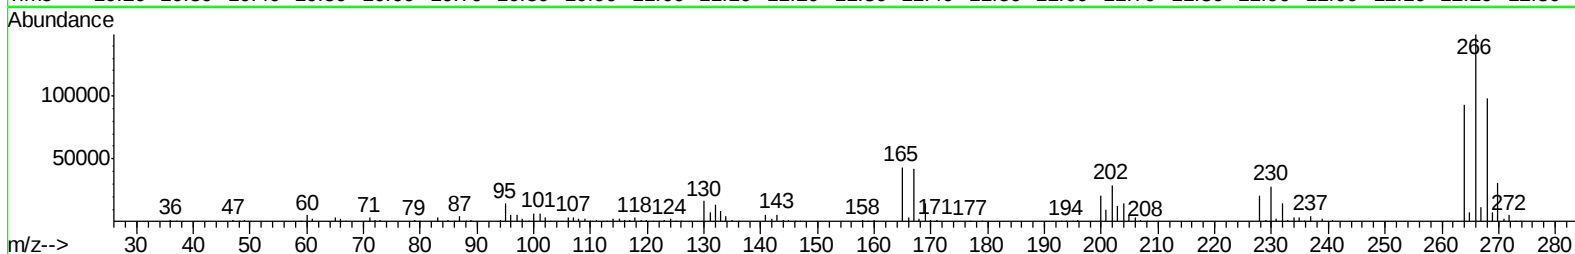


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF121315\
 Data File : BF083751.D
 Acq On : 14 Dec 2015 1:27
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 14 07:35:46 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121315.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 14 01:30:12 2015
 Response via : Initial Calibration

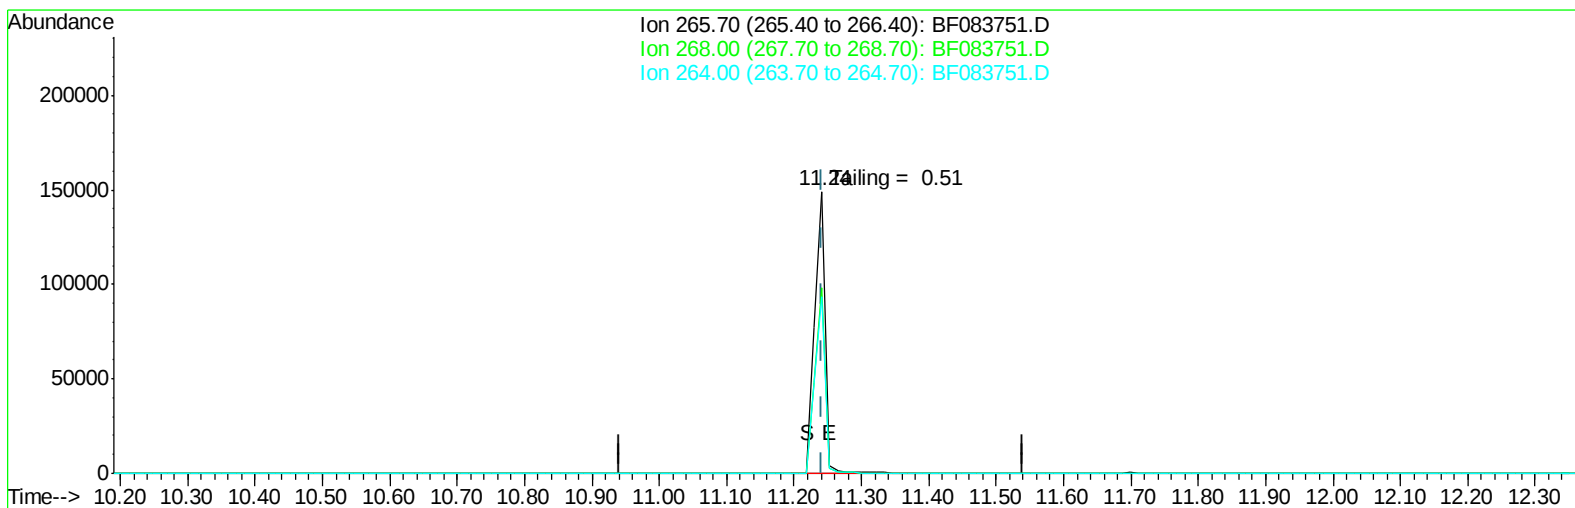

TIC: BF083751.D

(69) Pentachlorophenol (C)




11.242min (+0.001) 0.00ng

response 161246

Ion	Exp%	Act%
265.70	100	100
268.00	62.70	65.77
264.00	64.30	62.70
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF121315\
 Data File : BF083751.D
 Acq On : 14 Dec 2015 1:27
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 14 07:35:46 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121315.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 14 01:30:12 2015
 Response via : Initial Calibration

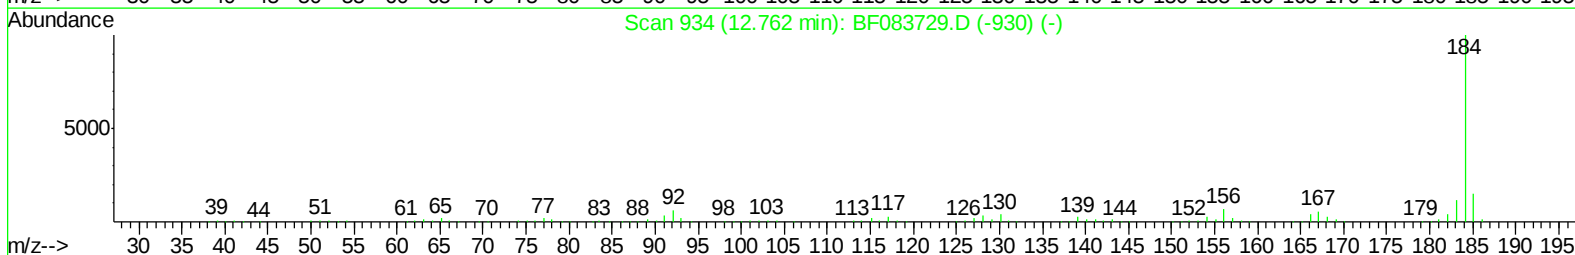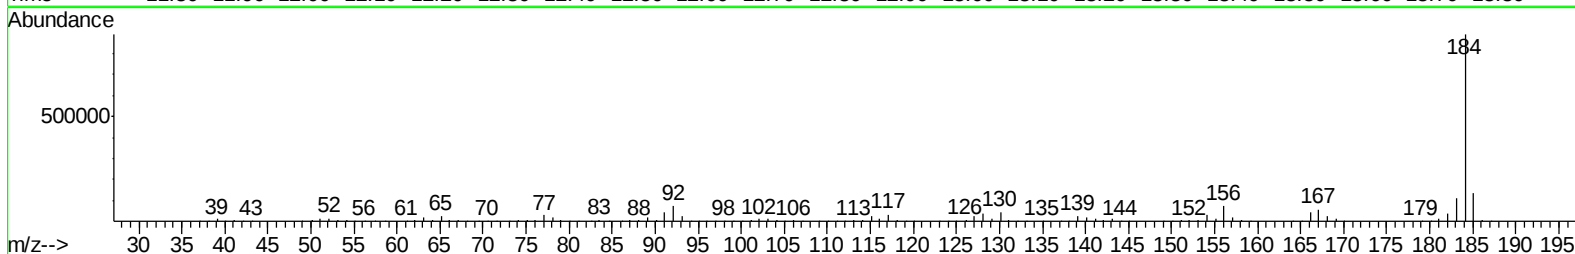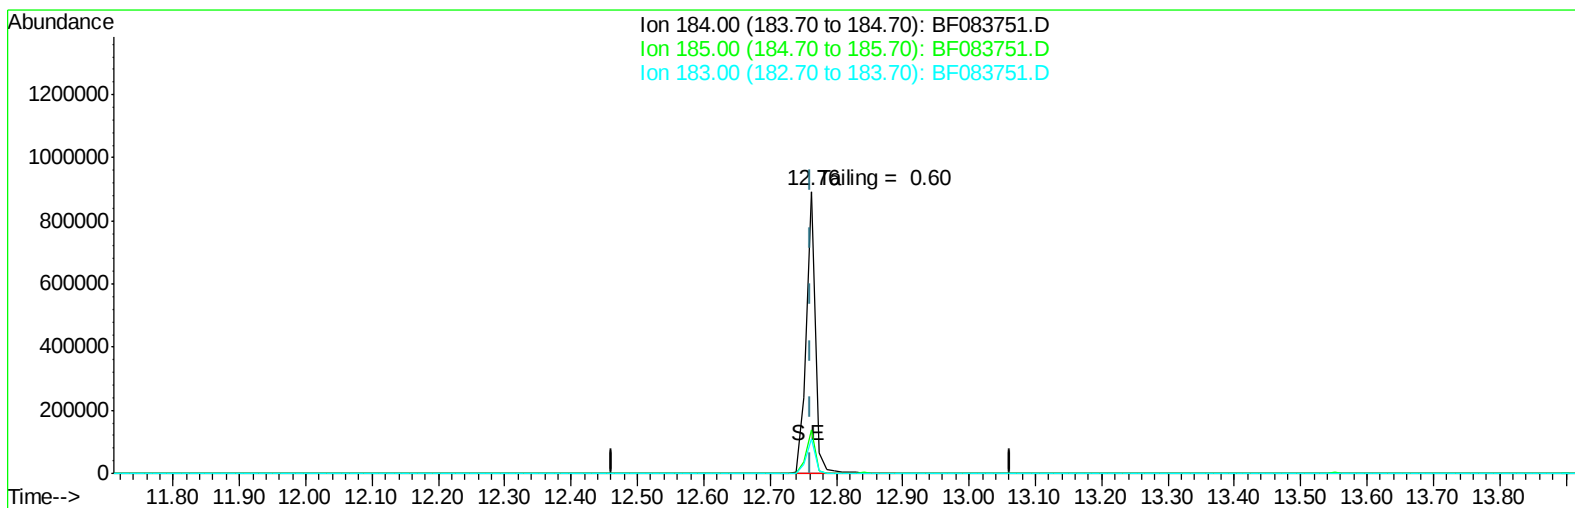

TIC: BF083751.D

(76) Benzidine

12.762min (-0.000) 112606.46ng

response 850990

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	15.32
183.00	11.20	12.45
0.00	0.00	0.00