


Data Path : Z:\HPCHEM1\BNA F\DATA\BF121315\
 Data File : BF083725.D
 Acq On : 13 Dec 2015 12:28
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 14 01:30:12 2015

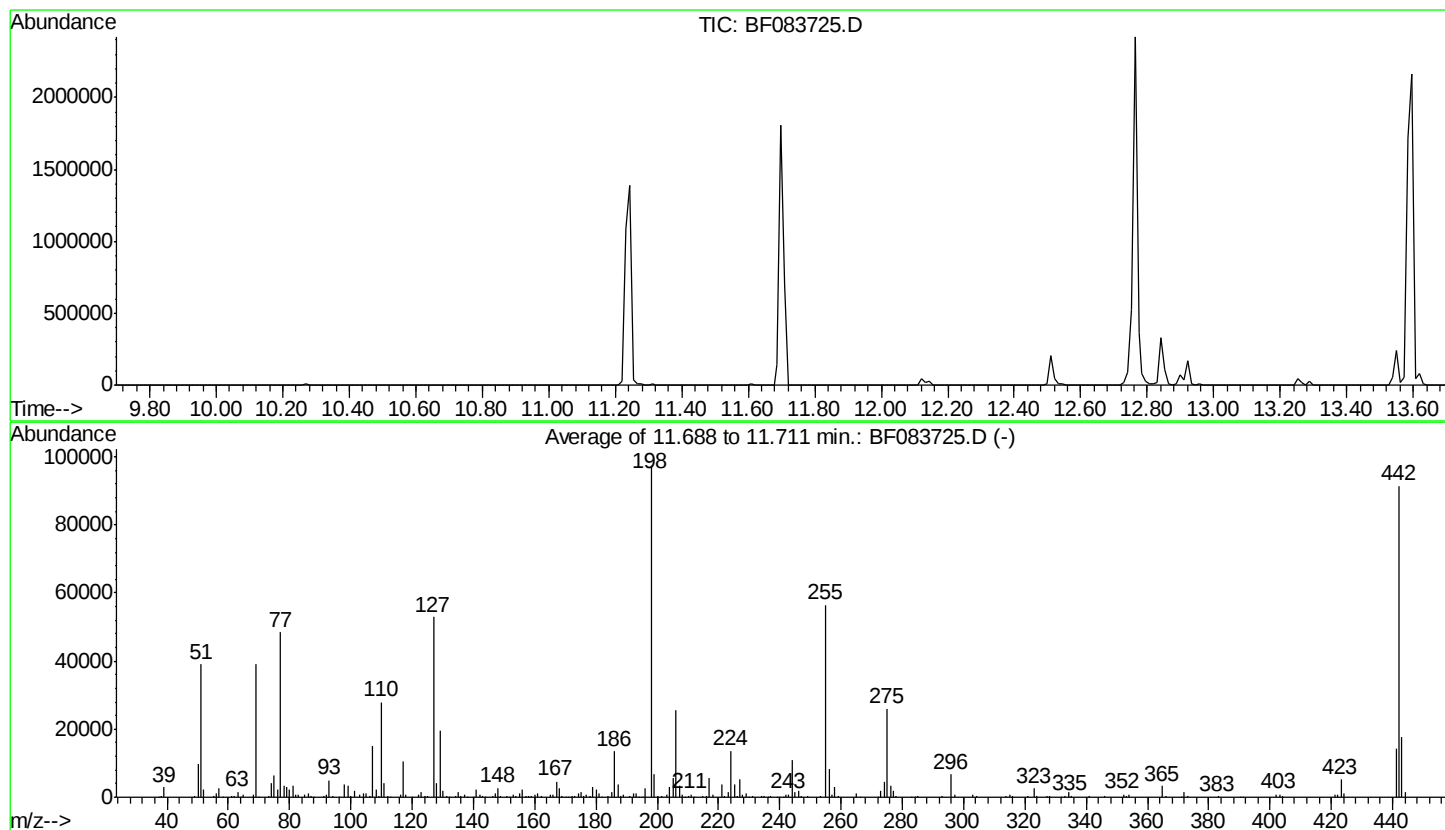

AutoFind: Scans 840, 841, 842; Background Corrected with Scan 837

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.1	39082	PASS
68	69	0.00	2	1.9	732	PASS
69	198	0.00	100	40.1	39100	PASS
70	69	0.00	2	0.3	131	PASS
127	198	10	80	54.4	52994	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	97418	PASS
199	198	5	9	6.9	6770	PASS
275	198	10	60	26.7	25992	PASS
365	198	1	100	3.4	3267	PASS
441	442	0.01	24	15.6	14328	PASS
442	198	50	100	94.0	91579	PASS
443	442	15	24	19.2	17608	PASS