


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF121315\
 Data File : BF083734.D
 Acq On : 13 Dec 2015 17:33
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 14 01:30:12 2015

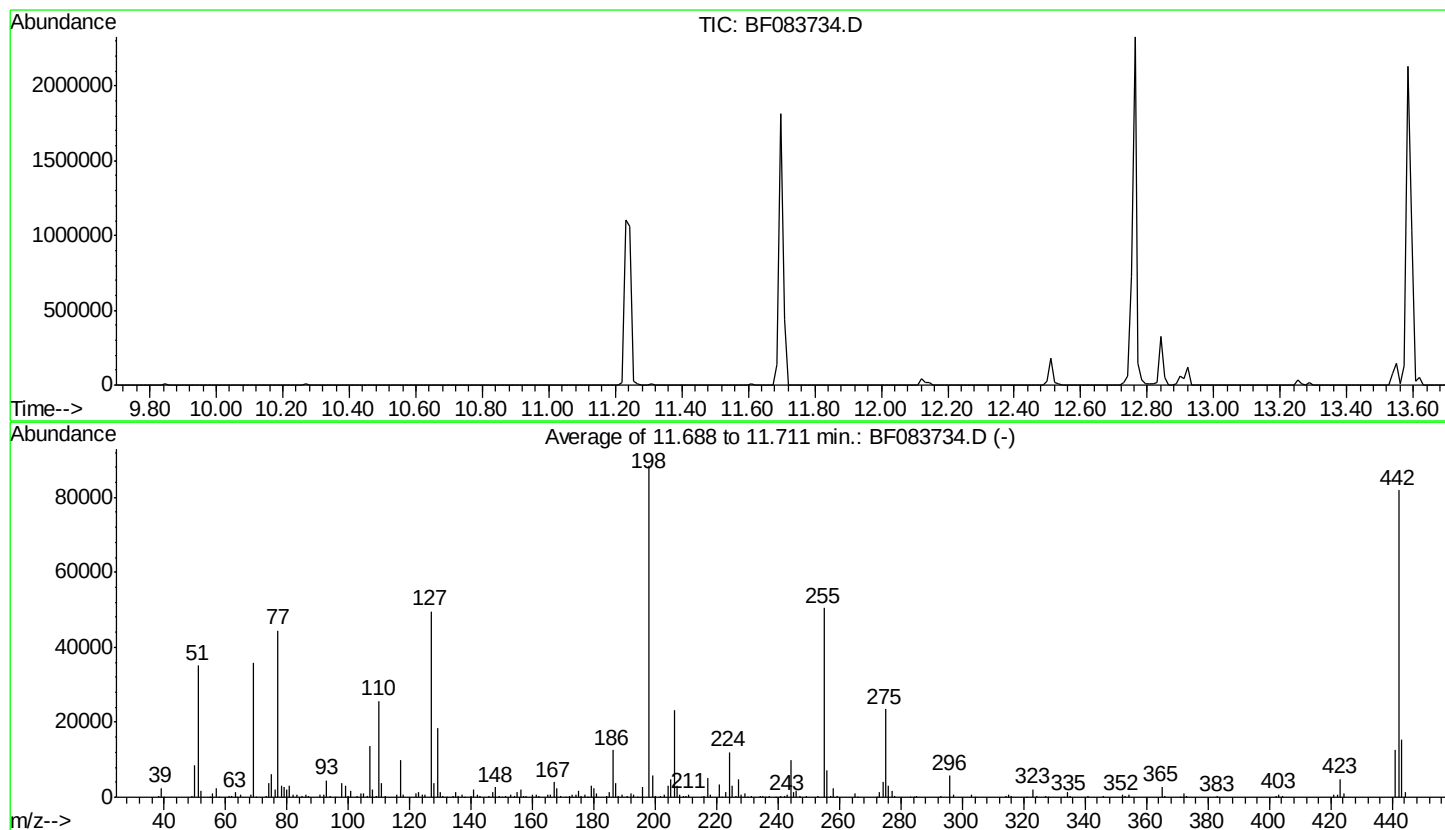

AutoFind: Scans 840, 841, 842; Background Corrected with Scan 837

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.7	35144	PASS
68	69	0.00	2	1.9	694	PASS
69	198	0.00	100	40.6	35922	PASS
70	69	0.00	2	0.4	139	PASS
127	198	10	80	56.2	49659	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	88424	PASS
199	198	5	9	6.8	5975	PASS
275	198	10	60	26.6	23550	PASS
365	198	1	100	3.2	2806	PASS
441	442	0.01	24	15.5	12726	PASS
442	198	50	100	92.6	81900	PASS
443	442	15	24	18.6	15228	PASS