


Data Path : Z:\HPCHEM1\BNA F\DATA\BF121315\
 Data File : BF083751.D
 Acq On : 14 Dec 2015 1:27
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 14 01:30:12 2015

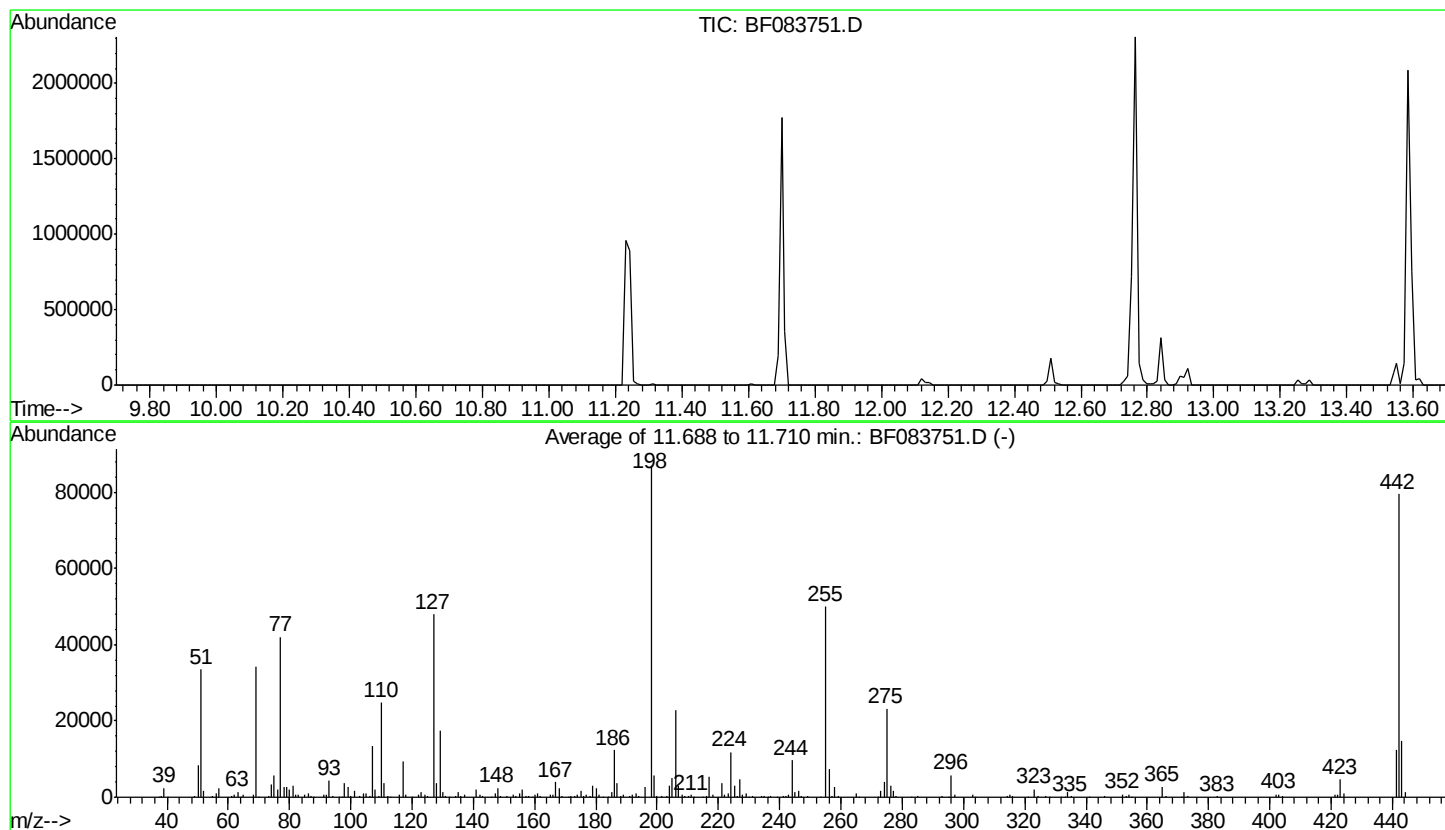

AutoFind: Scans 840, 841, 842; Background Corrected with Scan 837

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.5	33537	PASS
68	69	0.00	2	2.0	703	PASS
69	198	0.00	100	39.5	34377	PASS
70	69	0.00	2	0.5	165	PASS
127	198	10	80	55.2	47992	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	87013	PASS
199	198	5	9	6.6	5721	PASS
275	198	10	60	26.7	23244	PASS
365	198	1	100	3.2	2821	PASS
441	442	0.01	24	15.7	12526	PASS
442	198	50	100	91.4	79532	PASS
443	442	15	24	18.5	14722	PASS