
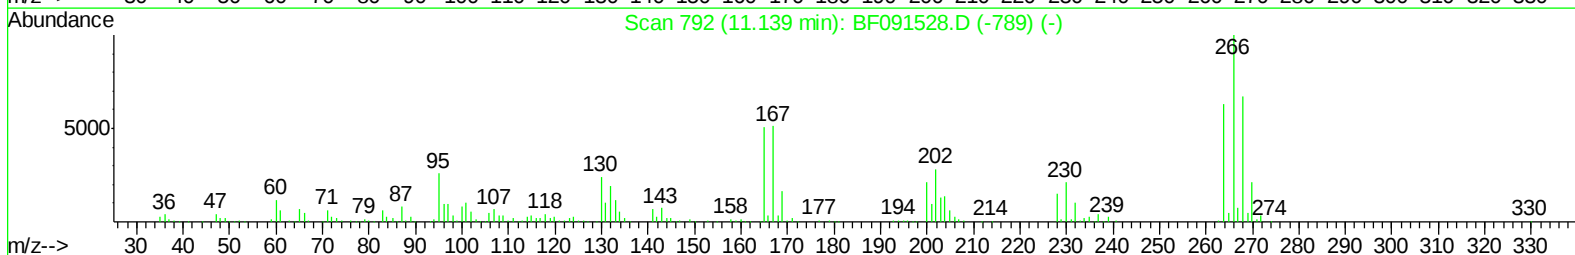
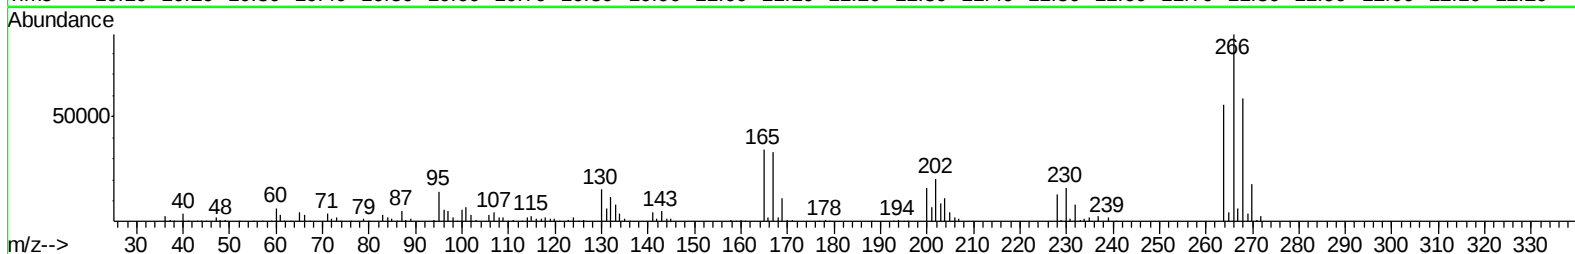


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF121316\
Data File : BF091545.D
Acq On : 13 Dec 2016 10:49
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 13 12:19:37 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF120916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 09 19:00:21 2016
Response via : Initial Calibration

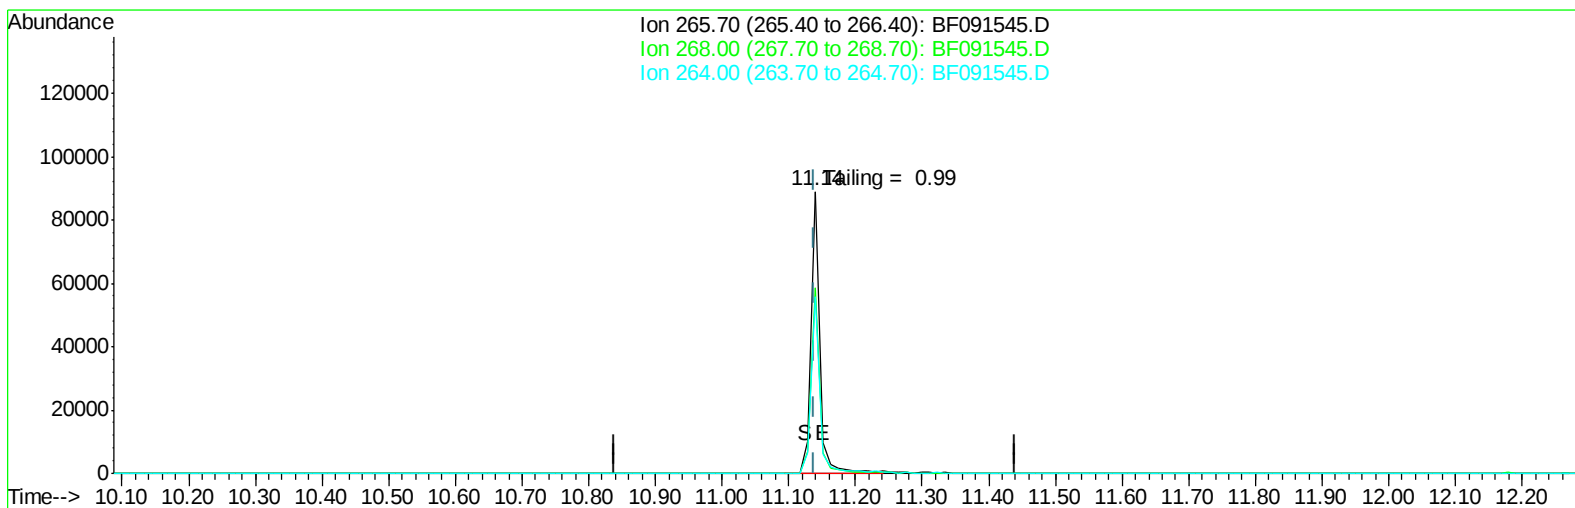

TIC: BF091545.D

(69) Pentachlorophenol (C)




11.139min (-0.000) 9253.50ng

response 82111

Ion	Exp%	Act%
265.70	100	100
268.00	62.90	65.85
264.00	60.20	62.66
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF121316\
Data File : BF091545.D
Acq On : 13 Dec 2016 10:49
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 13 12:19:37 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF120916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 09 19:00:21 2016
Response via : Initial Calibration

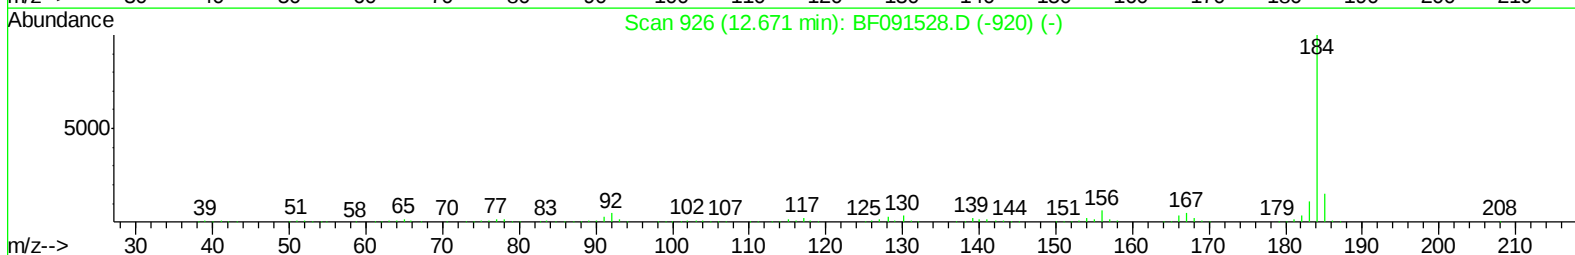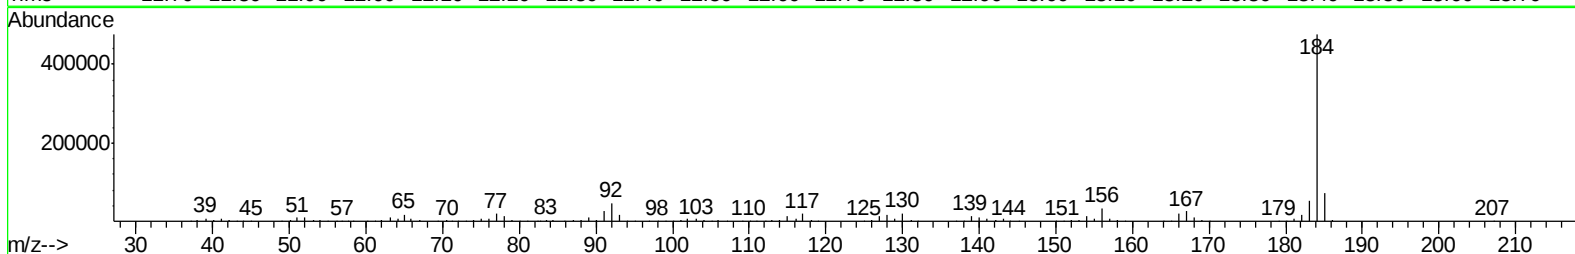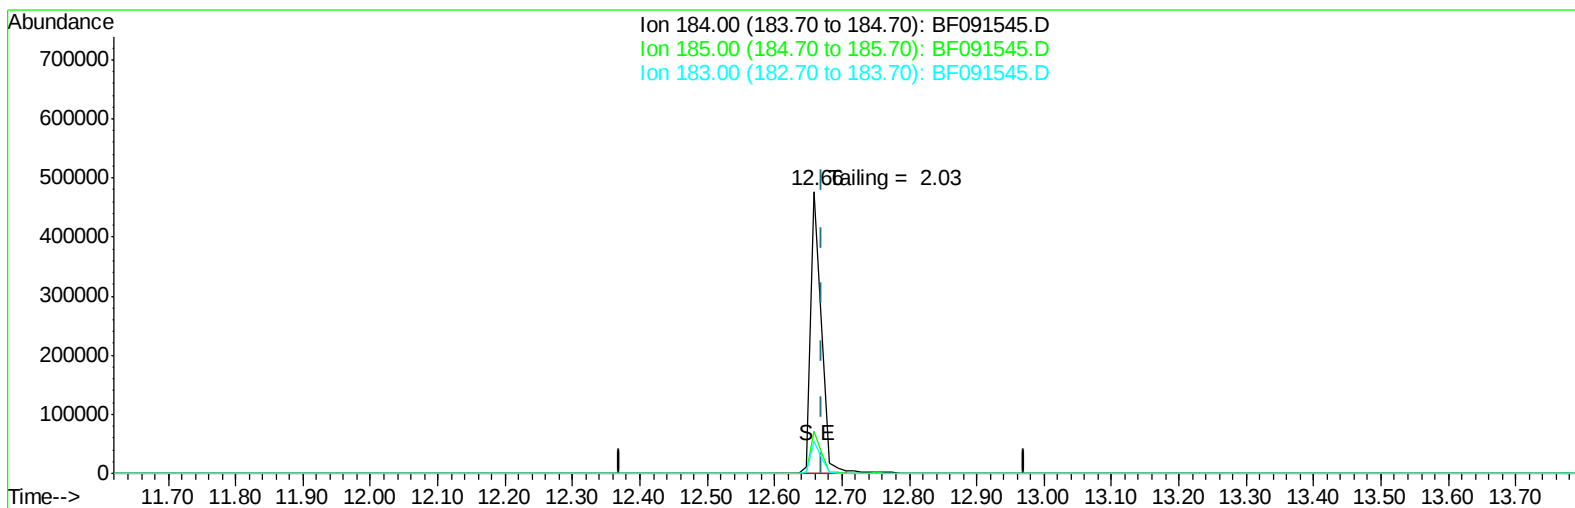

TIC: BF091545.D

(76) Benzidine

12.659min (-0.012) 3129.24ng

response 533905

Ion	Exp%	Act%
184.00	100	100
185.00	16.40	15.05
183.00	11.10	11.18
0.00	0.00	0.00