
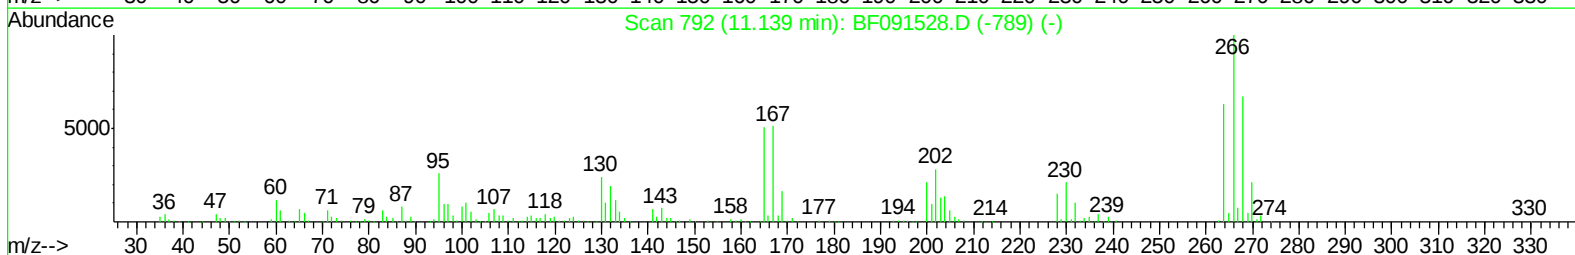
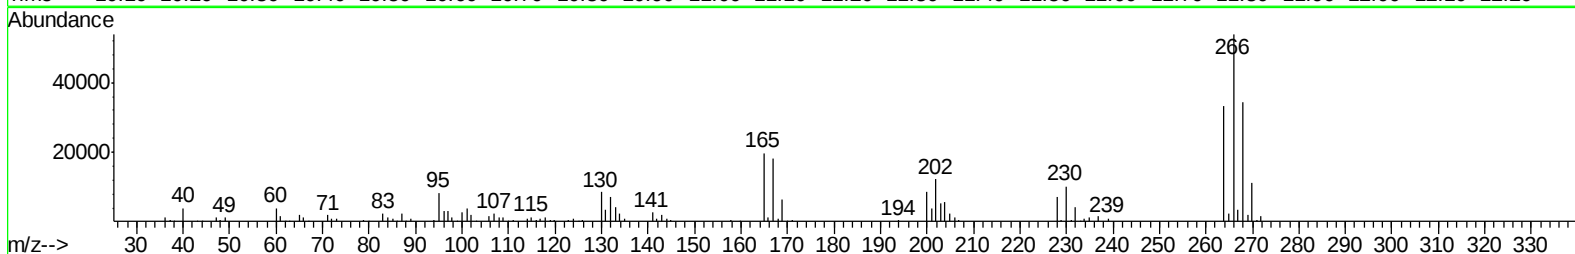


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF121316\
Data File : BF091570.D
Acq On : 14 Dec 2016 00:33
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 14 08:14:20 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF120916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 09 19:00:21 2016
Response via : Initial Calibration

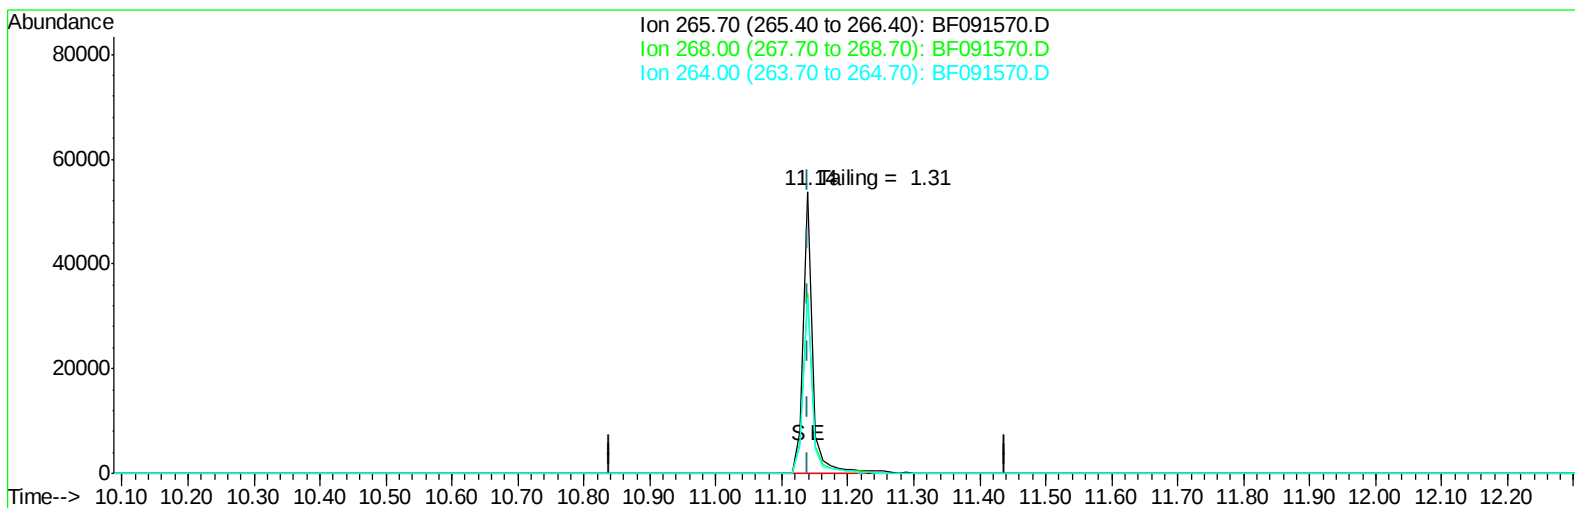

TIC: BF091570.D

(69) Pentachlorophenol (C)




11.139min (-0.000) 30807.48ng m

response 52493

Ion	Exp%	Act%
265.70	100	100
268.00	62.90	64.06
264.00	60.20	62.14
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF121316\
Data File : BF091570.D
Acq On : 14 Dec 2016 00:33
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 14 08:14:20 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF120916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 09 19:00:21 2016
Response via : Initial Calibration

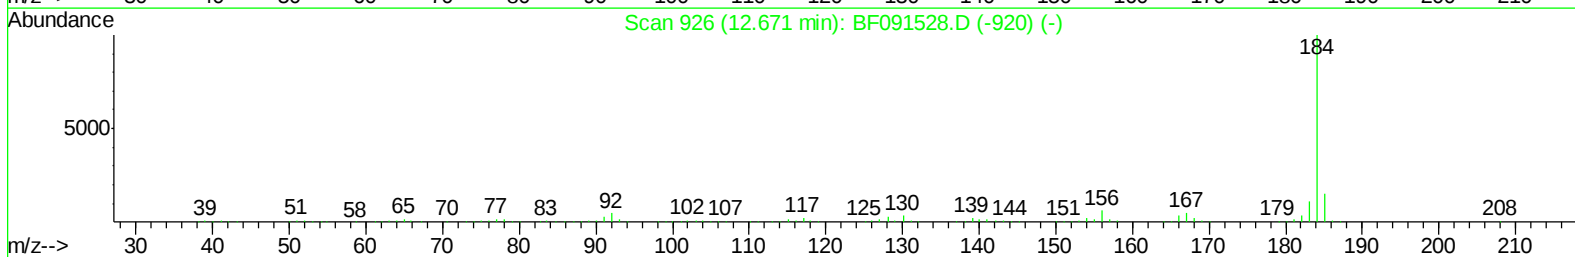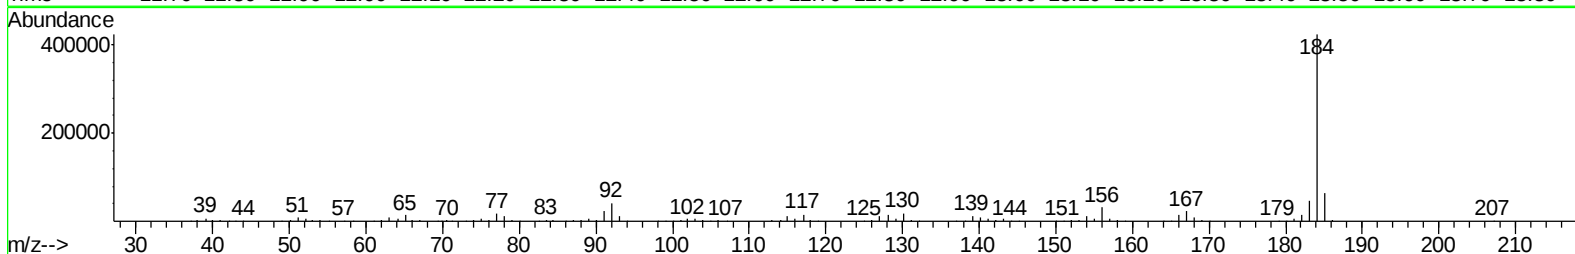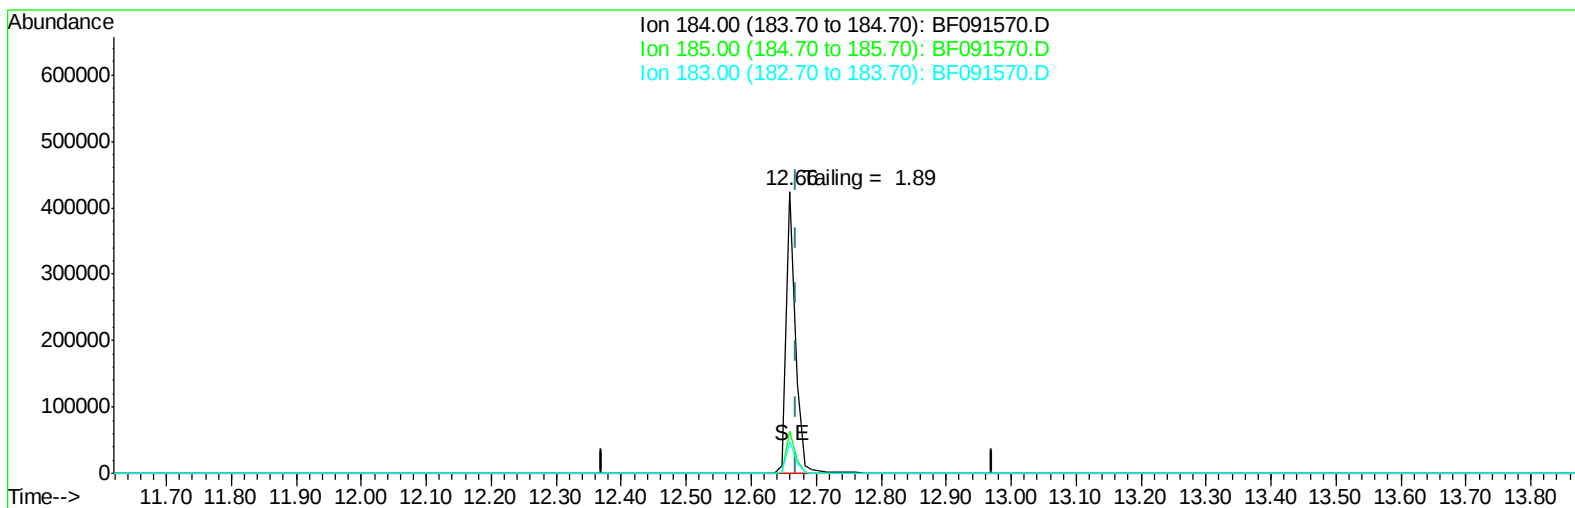

TIC: BF091570.D

(76) Benzidine

12.659min (-0.012) 0.00ng

response 415319

Ion	Exp%	Act%
184.00	100	100
185.00	16.40	15.24
183.00	11.10	11.24
0.00	0.00	0.00