


Data Path : Z:\HPCHEM1\BNA F\DATA\BF121316\
 Data File : BF091545.D
 Acq On : 13 Dec 2016 10:49
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF120916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 09 19:00:21 2016

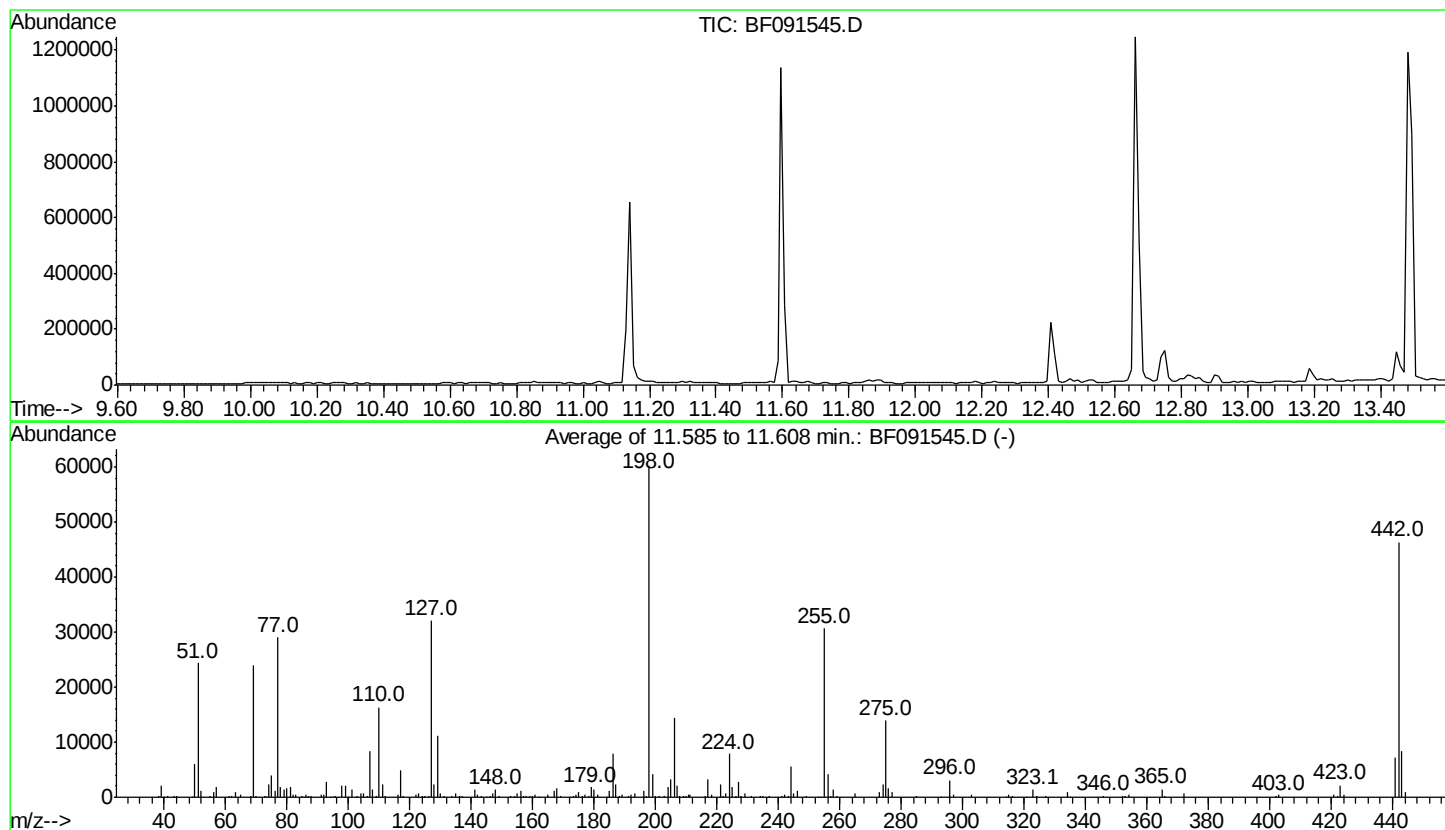

AutoFind: Scans 831, 832, 833; Background Corrected with Scan 828

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.5	24402	PASS
68	69	0.00	2	1.5	350	PASS
69	198	0.00	100	39.9	24031	PASS
70	69	0.00	2	0.6	154	PASS
127	198	10	80	53.3	32077	PASS
197	198	0.00	2	0.5	330	PASS
198	198	100	100	100.0	60229	PASS
199	198	5	9	7.1	4274	PASS
275	198	10	60	23.0	13873	PASS
365	198	1	100	2.5	1492	PASS
441	442	0.01	24	15.7	7280	PASS
442	198	50	100	76.9	46291	PASS
443	442	15	24	18.3	8469	PASS