


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF121316\
 Data File : BF091570.D
 Acq On : 14 Dec 2016 00:33
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF120916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 09 19:00:21 2016

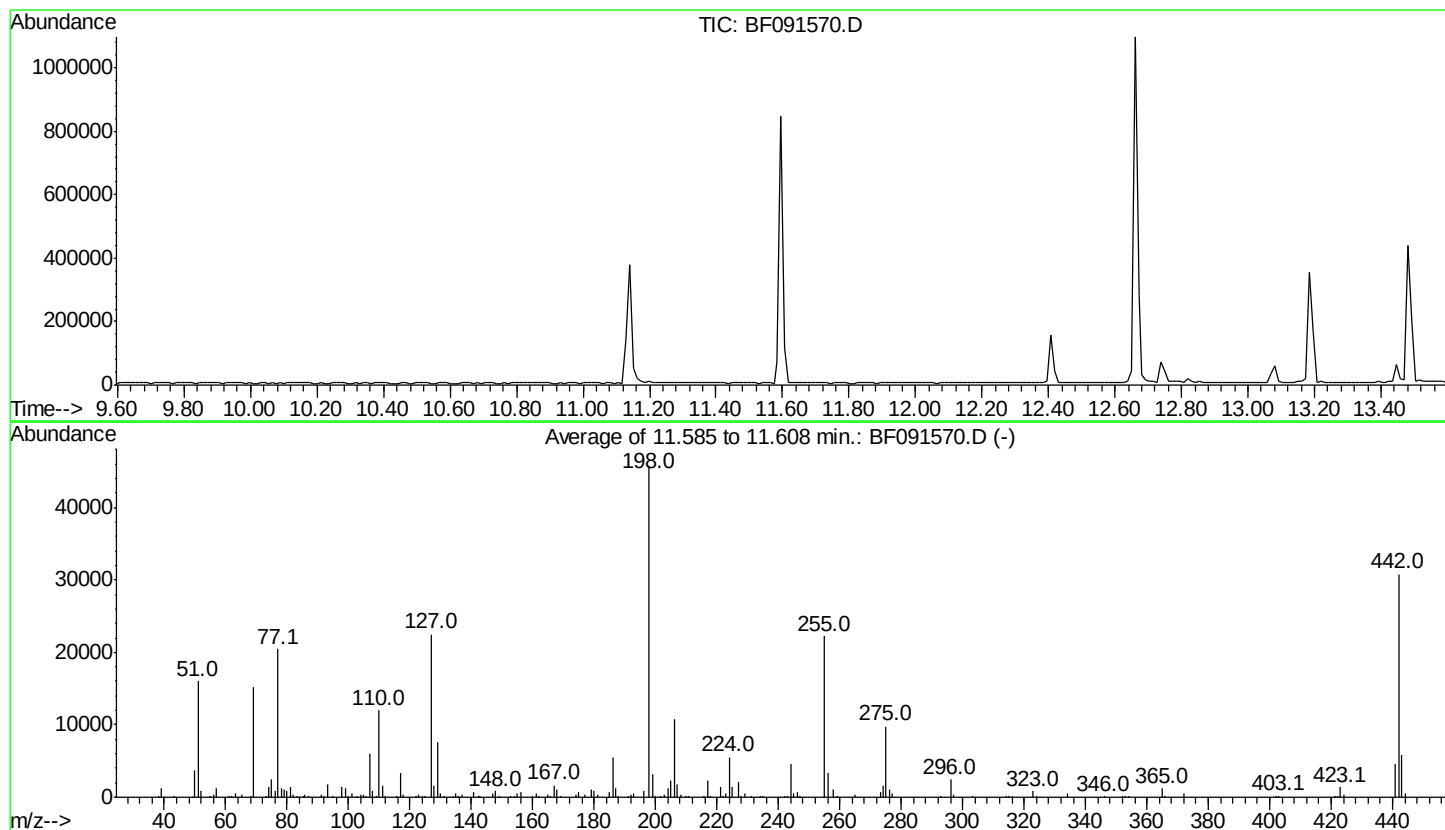

AutoFind: Scans 831, 832, 833; Background Corrected with Scan 828

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.0	15998	PASS
68	69	0.00	2	1.1	169	PASS
69	198	0.00	100	33.3	15242	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.1	22483	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	45767	PASS
199	198	5	9	6.8	3127	PASS
275	198	10	60	21.4	9811	PASS
365	198	1	100	2.6	1172	PASS
441	442	0.01	24	14.9	4568	PASS
442	198	50	100	67.2	30755	PASS
443	442	15	24	19.2	5914	PASS