

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF121317\
 Data File : BF101375.D
 Acq On : 13 Dec 2017 20:41
 Operator : SJ/JU
 Sample : I6816-02
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 120717-TIFR-F-D-M

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.034	498	501	514	rBV	75566	108281	2.16%	0.323%
2	5.440	566	570	590	rBV	1396441	1727075	34.41%	5.156%
3	5.716	601	617	619	rBV2	41803	134195	2.67%	0.401%
4	6.451	739	742	757	rBV	963740	1134997	22.61%	3.388%
5	6.587	761	765	772	rBV	2985903	2764685	55.08%	8.253%
6	6.816	800	804	811	rBV	1231420	1072522	21.37%	3.202%
7	6.975	826	831	834	rBV	3341059	3476706	69.27%	10.379%
8	7.351	887	895	896	rBV3	41850	75406	1.50%	0.225%
9	7.387	896	901	904	rBV	2787478	2926202	58.30%	8.735%
10	7.998	1000	1005	1014	rVB	94791	183091	3.65%	0.547%
11	8.098	1014	1022	1027	rVV	1482749	1459076	29.07%	4.356%
12	8.145	1027	1030	1039	rVB8	68868	142603	2.84%	0.426%
13	8.586	1098	1105	1110	rVB2	31141	60912	1.21%	0.182%
14	8.657	1110	1117	1125	rBV	108185	122222	2.44%	0.365%
15	8.851	1145	1150	1163	rVB9	22963	66592	1.33%	0.199%
16	9.075	1185	1188	1193	rVB	47612	55431	1.10%	0.165%
17	9.175	1199	1205	1208	rBV	4574911	5019115	100.00%	14.983%
18	9.816	1309	1314	1316	rBV	127936	147065	2.93%	0.439%
19	9.857	1316	1321	1328	rVB	1692309	1646617	32.81%	4.916%
20	9.975	1337	1341	1344	rVB	71457	75332	1.50%	0.225%
21	10.228	1380	1384	1389	rVB2	49335	64069	1.28%	0.191%
22	10.498	1427	1430	1433	rBV	58218	57936	1.15%	0.173%
23	10.569	1438	1442	1445	rVV	379628	325466	6.48%	0.972%
24	10.604	1445	1448	1452	rVV	165685	157637	3.14%	0.471%
25	10.651	1452	1456	1469	rVV	1725123	1691997	33.71%	5.051%
26	10.769	1473	1476	1482	rVB	42370	66335	1.32%	0.198%
27	11.027	1518	1520	1522	rBV	47913	50973	1.02%	0.152%
28	11.157	1538	1542	1547	rBV2	139995	141531	2.82%	0.423%
29	11.351	1570	1575	1578	rBV	1617517	1549867	30.88%	4.627%
30	11.380	1578	1580	1583	rVB	91478	77033	1.53%	0.230%
31	11.639	1622	1624	1627	rVB2	88703	73331	1.46%	0.219%
32	11.822	1652	1655	1659	rVB	126252	108357	2.16%	0.323%
33	12.063	1692	1696	1698	rBV	114020	96356	1.92%	0.288%
34	12.222	1719	1723	1727	rVB	58246	53179	1.06%	0.159%

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF121317\
Data File : BF101375.D
Acq On : 13 Dec 2017 20:41
Operator : SJ/JU
Sample : I6816-02
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
120717-TIFR-F-D-M

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	12.939	1839	1845	1848	rVB	3926067	4116463	82.02%	12.289%
36	13.945	2011	2016	2021	rVB	154471	172617	3.44%	0.515%
37	13.998	2021	2025	2033	rBV	1183772	1090562	21.73%	3.256%
38	14.815	2158	2164	2169	rVB	180217	245088	4.88%	0.732%
39	15.474	2269	2276	2283	rBV	649983	890850	17.75%	2.659%
40	16.457	2438	2443	2444	rBV5	55596	70319	1.40%	0.210%


Sum of corrected areas: 33498091

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF121317\
Data File : BF101375.D
Acq On : 13 Dec 2017 20:41
Operator : SJ/JU
Sample : I6816-02
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
120717-TIFR-F-D-M

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

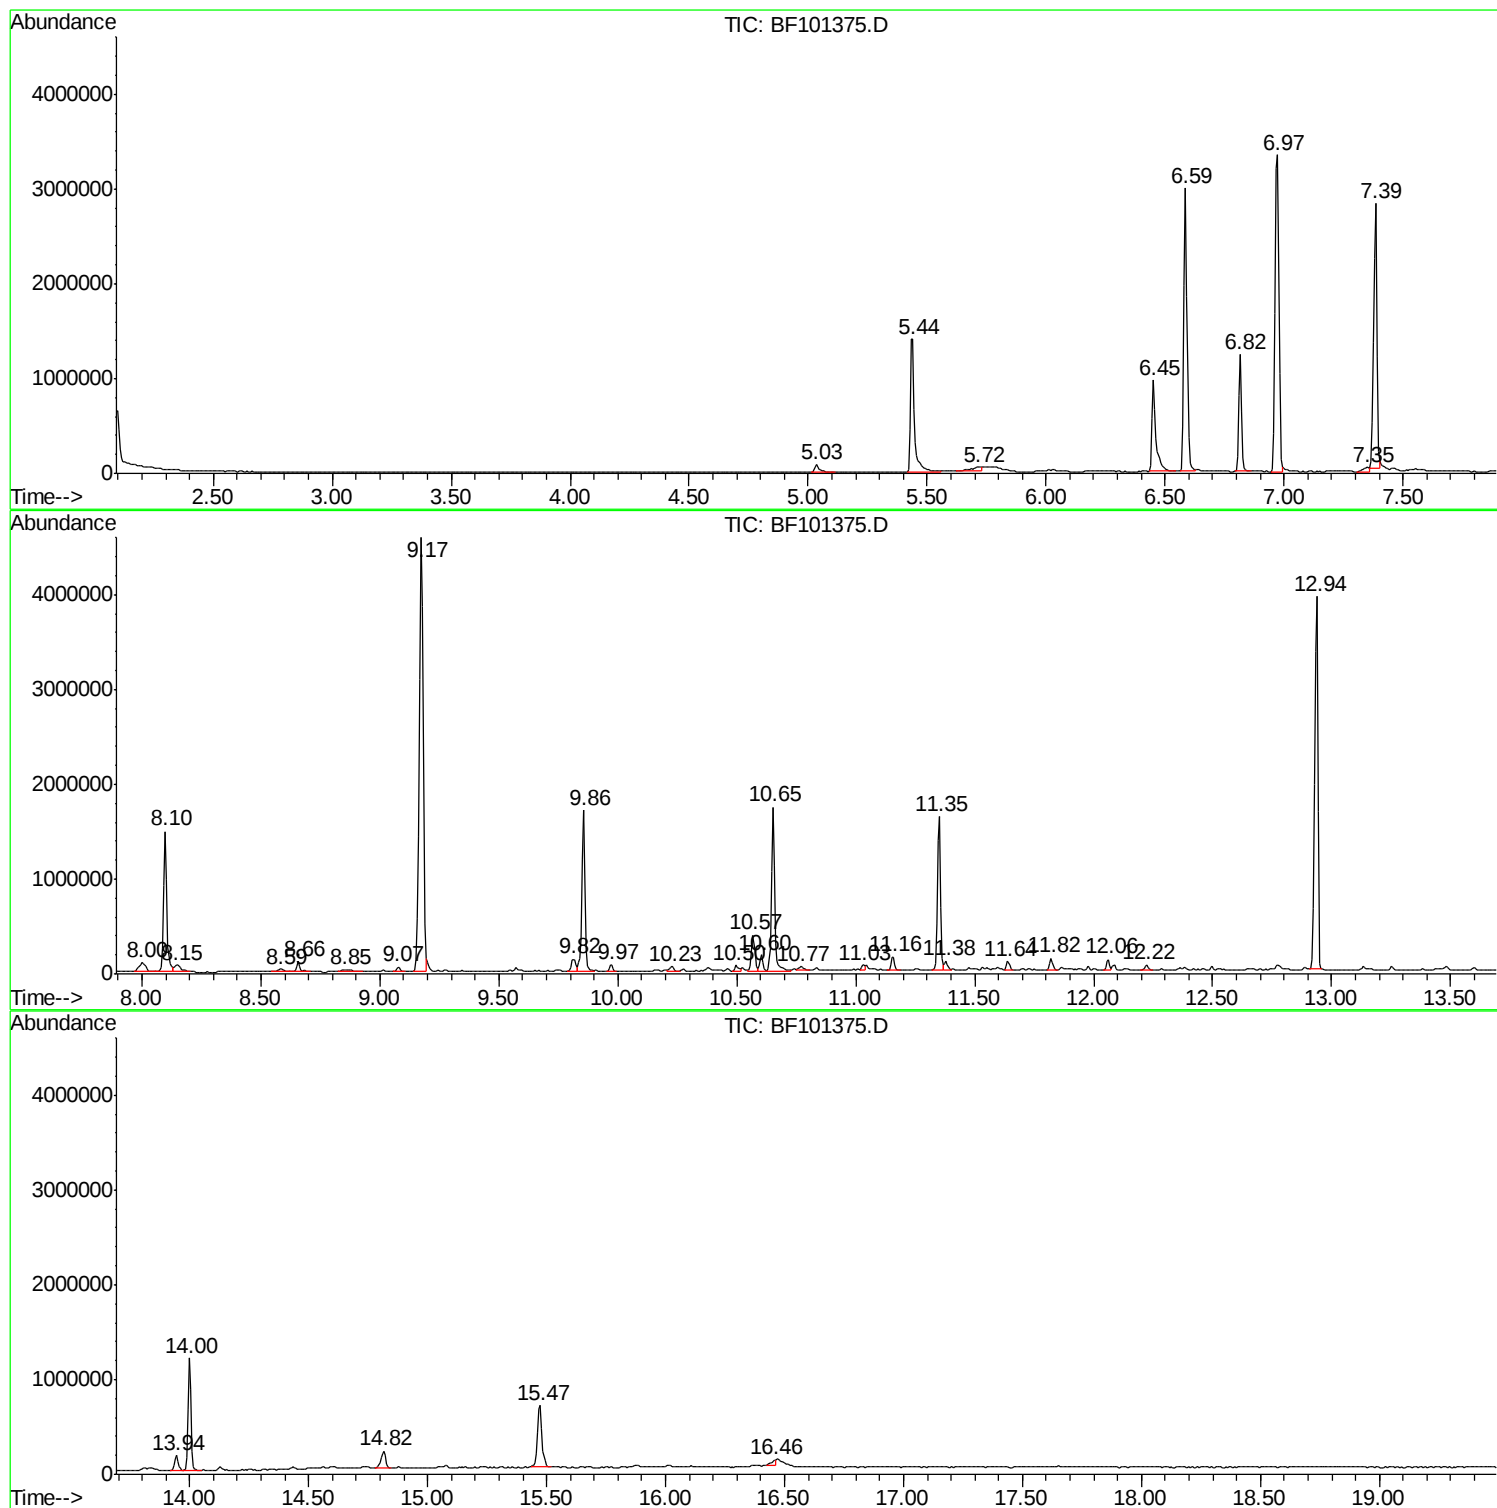

Data_Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF121317\
Data_File : BF101375.D
Acq_On : 13-Dec-2017 20:411
Operator : SJ/JUU
Sample : I6816-022
Misc :
ALS_Vial : 3 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
120717-TIFR-F-D-M

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
