

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF121317\
 Data File : BF101376.D
 Acq On : 13 Dec 2017 21:08
 Operator : SJ/JU
 Sample : I6816-03
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 120717-TIFR-F-D-S

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.040	499	502	516	rBV	48460	74663	1.49%	0.234%
2	5.439	566	570	594	rBV	1449583	1825990	36.34%	5.716%
3	6.451	738	742	761	rBV	1011843	1243024	24.74%	3.891%
4	6.586	761	765	772	rBV	3029120	2801108	55.74%	8.769%
5	6.816	800	804	814	rBV	1216177	1087426	21.64%	3.404%
6	6.975	826	831	834	rBV	3291314	3510818	69.86%	10.991%
7	7.386	895	901	904	rBV	2876327	3012894	59.96%	9.432%
8	8.098	1018	1022	1034	rVB	1497830	1441597	28.69%	4.513%
9	8.657	1112	1117	1126	rBV	155039	165188	3.29%	0.517%
10	9.175	1199	1205	1208	rBV	4540136	5025182	100.00%	15.732%
11	9.575	1267	1273	1277	rBV	57507	63621	1.27%	0.199%
12	9.857	1314	1321	1336	rVB	1617730	1632679	32.49%	5.111%
13	10.569	1438	1442	1448	rVB	581314	486419	9.68%	1.523%
14	10.651	1452	1456	1470	rBV	1745644	1714384	34.12%	5.367%
15	10.774	1474	1477	1484	rVB2	31917	51533	1.03%	0.161%
16	11.351	1570	1575	1582	rVB	1559672	1546605	30.78%	4.842%
17	12.939	1839	1845	1848	rBV	3944531	4193599	83.45%	13.128%
18	13.833	1992	1997	2007	rBV7	38196	88885	1.77%	0.278%
19	13.998	2021	2025	2032	rBV	1186854	1111309	22.11%	3.479%
20	15.474	2270	2276	2286	rVB	655606	866321	17.24%	2.712%


Sum of corrected areas: 31943245

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF121317\
Data File : BF101376.D
Acq On : 13 Dec 2017 21:08
Operator : SJ/JU
Sample : I6816-03
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
120717-TIFR-F-D-S

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

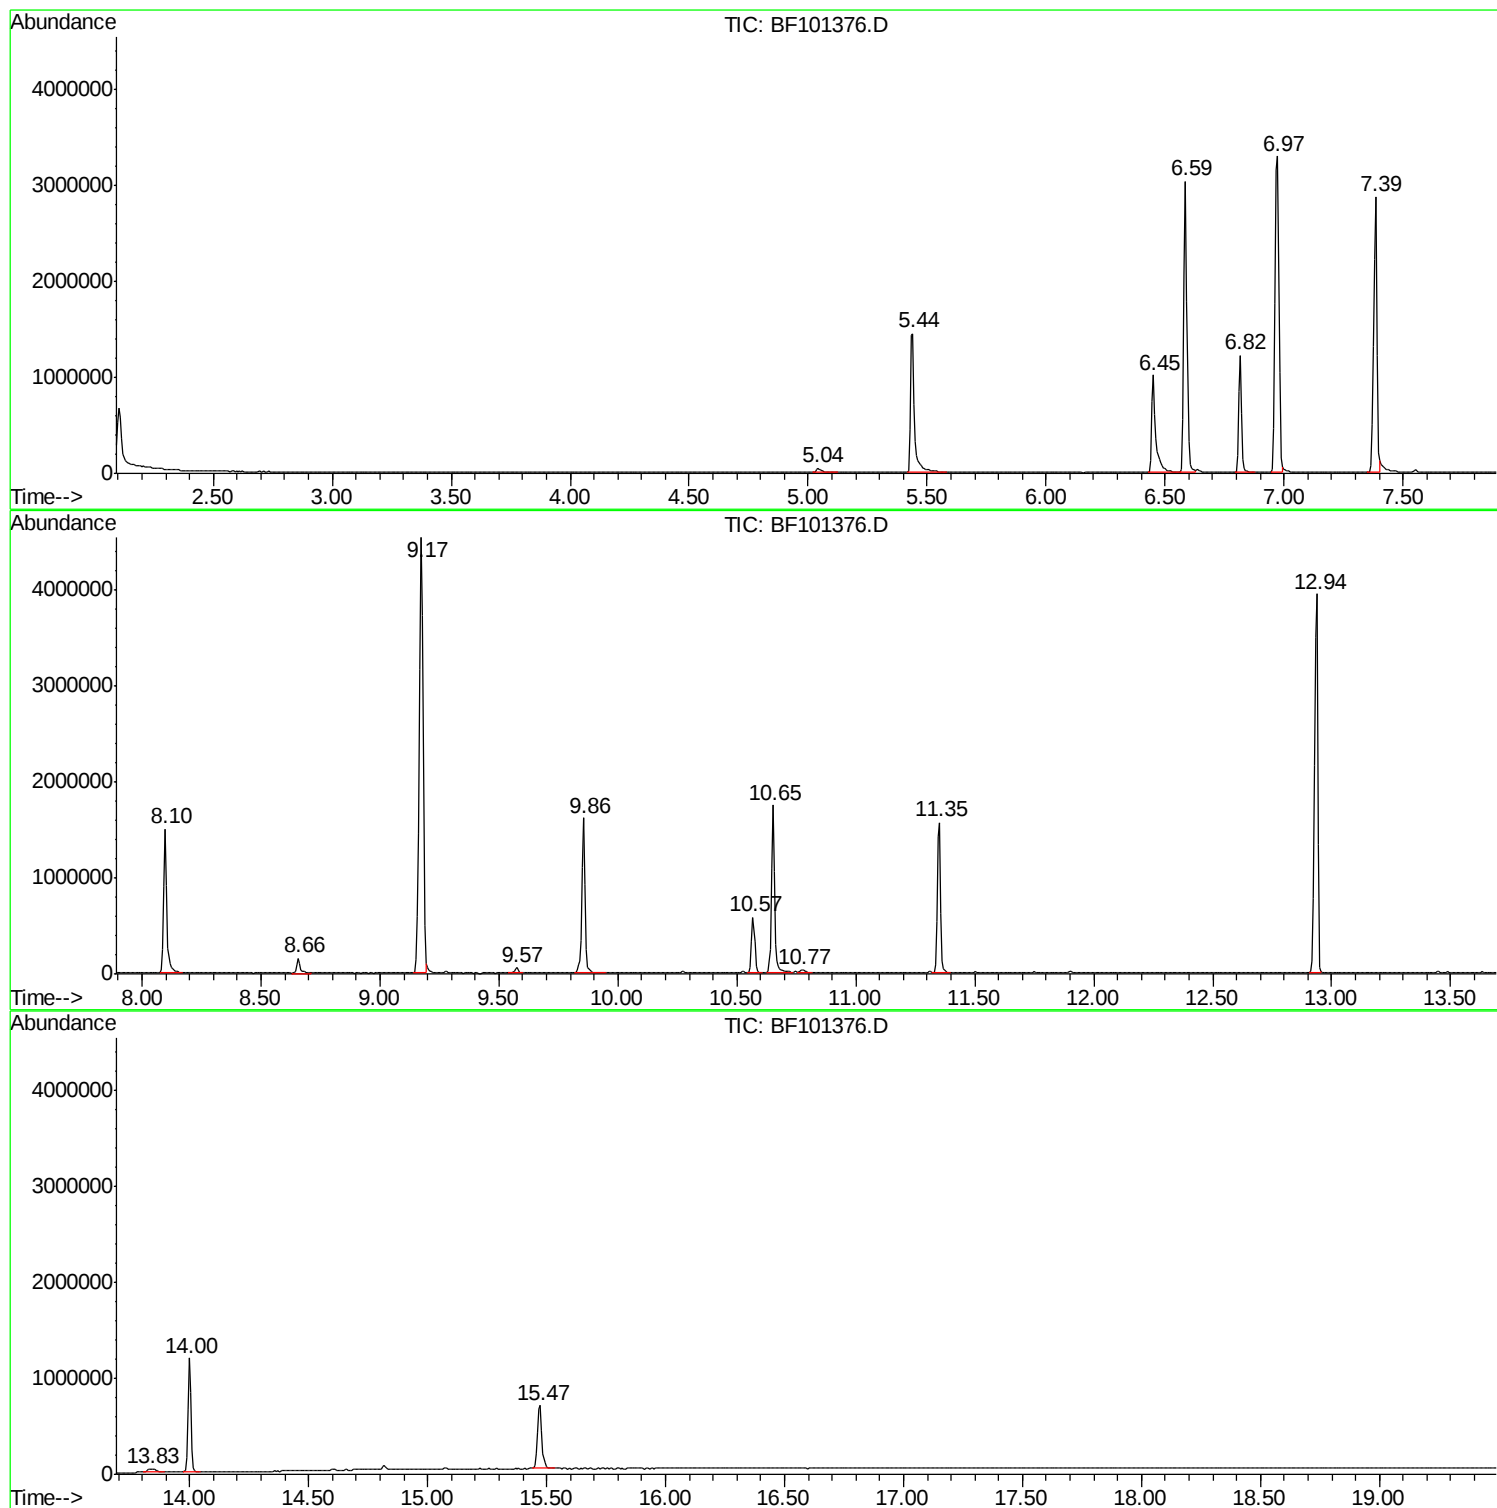

Data_Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF121317\
Data_File : BF101376.D
Acq_On : 13-Dec-2017 21:088
Operator : SJ/JUU
Sample : I6816-033
Misc :
ALS_Vial : 4 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
120717-TIFR-F-D-S

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
