

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF121317\
 Data File : BF101378.D
 Acq On : 13 Dec 2017 22:01
 Operator : SJ/JU
 Sample : I6816-05
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 120717-TIFR-F-U-M

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.040	499	502	516	rBV	66893	110381	2.06%	0.331%
2	5.434	566	569	587	rBV	1610121	1960085	36.51%	5.876%
3	6.451	738	742	761	rBV	1125798	1368406	25.49%	4.102%
4	6.587	761	765	772	rBV	3263826	3020272	56.27%	9.054%
5	6.816	800	804	812	rBV	1213080	1065186	19.84%	3.193%
6	6.975	826	831	834	rBV	3604815	3797791	70.75%	11.385%
7	7.386	895	901	904	rBV	3008989	3308466	61.63%	9.918%
8	8.098	1018	1022	1038	rVB	1453429	1421567	26.48%	4.262%
9	8.657	1113	1117	1126	rBV	113836	120405	2.24%	0.361%
10	9.175	1199	1205	1209	rBV	4602165	5367910	100.00%	16.092%
11	9.857	1314	1321	1330	rVB	1567255	1566702	29.19%	4.697%
12	10.569	1438	1442	1449	rVB	394951	324311	6.04%	0.972%
13	10.651	1452	1456	1470	rBV	1901745	1916433	35.70%	5.745%
14	11.351	1570	1575	1582	rBV	1469397	1495498	27.86%	4.483%
15	12.939	1839	1845	1848	rBV	4086602	4463148	83.14%	13.380%
16	13.833	1992	1997	2005	rBV7	23984	64967	1.21%	0.195%
17	13.998	2021	2025	2033	rBV	1188393	1086721	20.24%	3.258%
18	15.468	2268	2275	2286	rVB	635999	899471	16.76%	2.696%


Sum of corrected areas: 33357720

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF121317\
Data File : BF101378.D
Acq On : 13 Dec 2017 22:01
Operator : SJ/JU
Sample : I6816-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
120717-TIFR-F-U-M

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

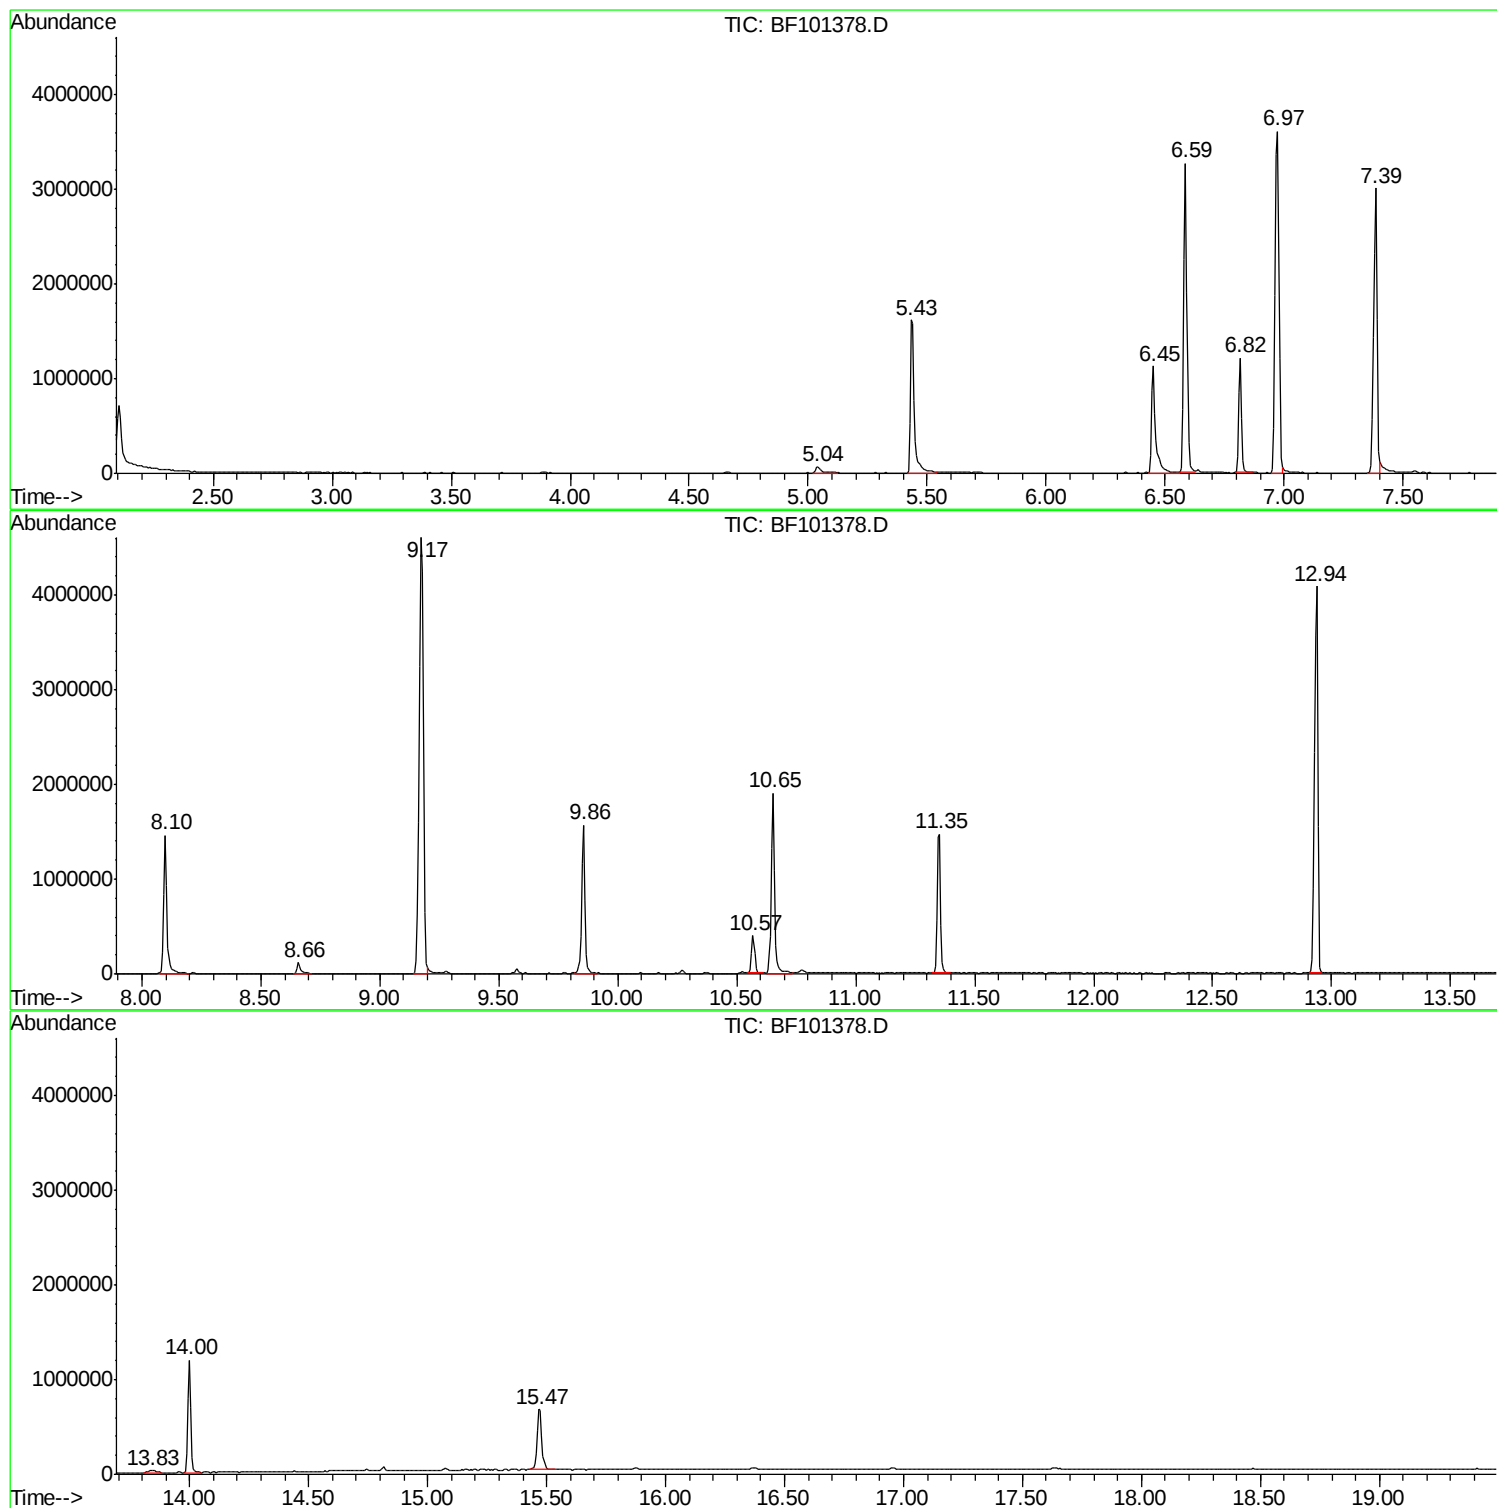

Data_Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF121317\
Data_File : BF101378.D
Acq_On : 13-Dec-2017 22:011
Operator : SJ/JUU
Sample : I6816-055
Misc :
ALS_Vial : 6 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
120717-TIFR-F-U-M

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
