

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF121317\
 Data File : BF101380.D
 Acq On : 13 Dec 2017 22:55
 Operator : SJ/JU
 Sample : I6816-07
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 120717-TIDO-F-D-B

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.034	498	501	509	rBV	85177	116121	2.31%	0.356%
2	5.434	566	569	589	rBV	1477019	1792050	35.70%	5.496%
3	6.451	738	742	761	rBV	967834	1215701	24.22%	3.729%
4	6.586	761	765	772	rBV	3041970	2825428	56.28%	8.666%
5	6.816	800	804	817	rBV	1204841	1072283	21.36%	3.289%
6	6.975	826	831	834	rBV	3362674	3540220	70.52%	10.858%
7	7.386	896	901	904	rBV	2837486	3066451	61.09%	9.405%
8	8.098	1018	1022	1039	rVB	1498443	1440804	28.70%	4.419%
9	8.657	1113	1117	1125	rBV	87342	100679	2.01%	0.309%
10	9.175	1199	1205	1208	rBV	4476152	5019965	100.00%	15.396%
11	9.857	1311	1321	1335	rBV	1568378	1592684	31.73%	4.885%
12	10.569	1438	1442	1448	rBV	350361	290492	5.79%	0.891%
13	10.651	1452	1456	1468	rBV	1796769	1803681	35.93%	5.532%
14	11.345	1570	1574	1583	rBV	1461260	1488438	29.65%	4.565%
15	12.939	1839	1845	1848	rBV	3805128	4142622	82.52%	12.705%
16	13.998	2021	2025	2034	rBV	1118160	1050402	20.92%	3.222%
17	14.745	2148	2152	2155	rBV	55875	55194	1.10%	0.169%
18	15.074	2204	2208	2212	rBV	97583	103905	2.07%	0.319%
19	15.468	2267	2275	2282	rBV2	621136	1010932	20.14%	3.101%
20	15.874	2339	2344	2350	rBV	147272	221360	4.41%	0.679%
21	16.368	2422	2428	2435	rBV	140777	251742	5.01%	0.772%
22	16.951	2521	2527	2536	rVB2	86202	179328	3.57%	0.550%
23	17.639	2637	2644	2655	rVB3	62867	151942	3.03%	0.466%
24	18.462	2779	2784	2794	rVB4	29463	72787	1.45%	0.223%


Sum of corrected areas: 32605211

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF121317\
Data File : BF101380.D
Acq On : 13 Dec 2017 22:55
Operator : SJ/JU
Sample : I6816-07
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
120717-TIDO-F-D-B

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

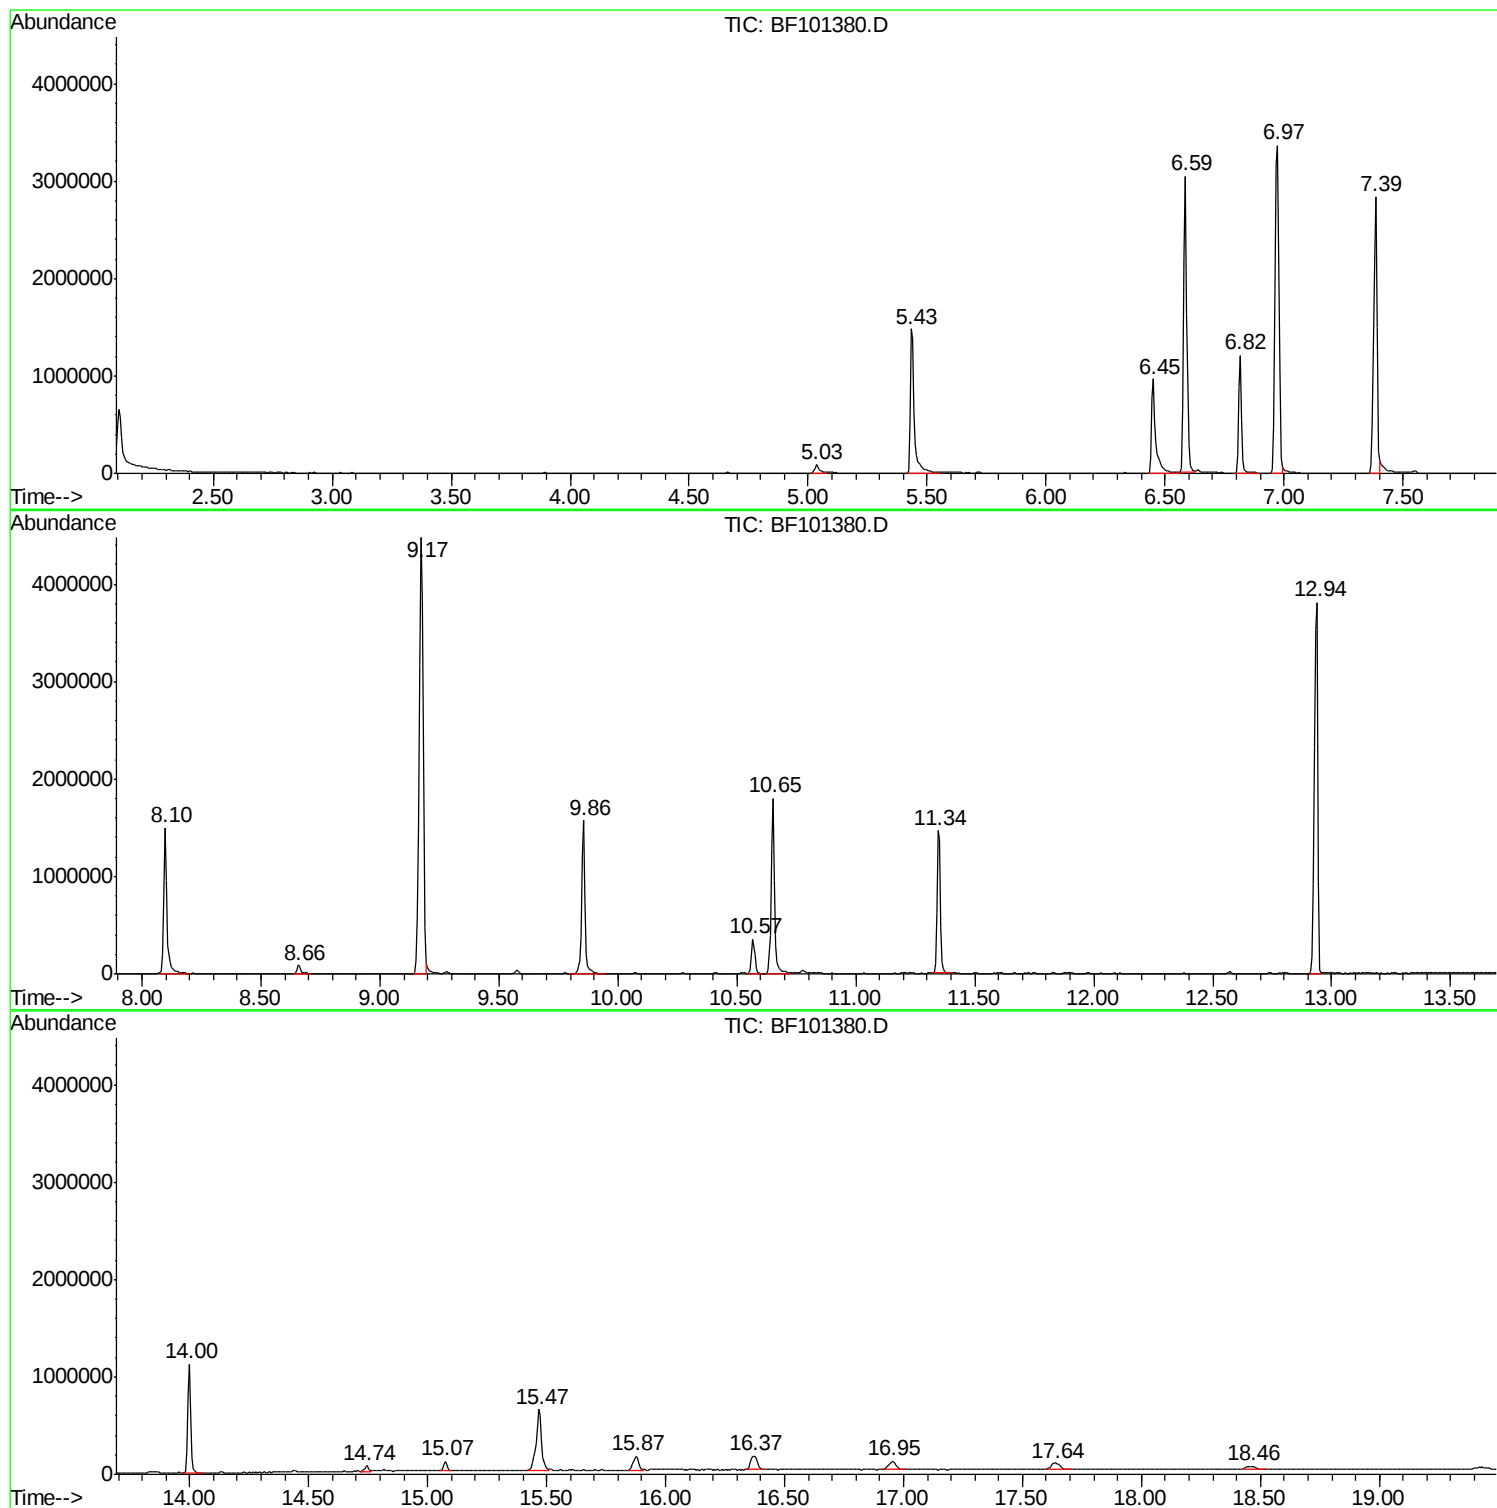

Data_Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF121317\
Data_File : BF101380.D
Acq_On : 13-Dec-2017 22:555
Operator : SJ/JUU
Sample : I6816-077
Misc :
ALS_Vial : 8 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
120717-TIDO-F-D-B

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
