

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF121317\
 Data File : BF101381.D
 Acq On : 13 Dec 2017 23:22
 Operator : SJ/JU
 Sample : I6816-08
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 120717-TIDO-F-D-S

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.034	498	501	514	rBV	61899	98524	2.19%	0.338%
2	5.434	566	569	593	rBV	1318551	1559014	34.68%	5.346%
3	6.451	738	742	761	rBV	787495	1050341	23.36%	3.602%
4	6.587	761	765	772	rBV	2634067	2499492	55.60%	8.571%
5	6.816	800	804	811	rBV	1099437	1028091	22.87%	3.525%
6	6.969	826	830	846	rBV	3040790	3200043	71.18%	10.973%
7	7.387	896	901	920	rBV	2565631	2837791	63.13%	9.731%
8	8.098	1018	1022	1037	rVB	1411546	1377945	30.65%	4.725%
9	8.657	1112	1117	1126	rBV	96899	110476	2.46%	0.379%
10	9.175	1199	1205	1208	rBV	4331171	4495453	100.00%	15.415%
11	9.575	1268	1273	1278	rBV	42434	47037	1.05%	0.161%
12	9.857	1314	1321	1333	rVB	1494415	1547174	34.42%	5.305%
13	10.569	1438	1442	1448	rBV	360612	309984	6.90%	1.063%
14	10.651	1452	1456	1471	rBV	1626881	1649007	36.68%	5.654%
15	11.345	1570	1574	1583	rBV	1527873	1475689	32.83%	5.060%
16	12.933	1839	1844	1847	rBV	3642257	3811802	84.79%	13.070%
17	13.833	1992	1997	2007	rBV5	49075	129986	2.89%	0.446%
18	13.998	2021	2025	2034	rBV	1091020	1073626	23.88%	3.681%
19	15.468	2268	2275	2285	rBV2	623936	862317	19.18%	2.957%


Sum of corrected areas: 29163792

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF121317\
Data File : BF101381.D
Acq On : 13 Dec 2017 23:22
Operator : SJ/JU
Sample : I6816-08
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
120717-TIDO-F-D-S

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

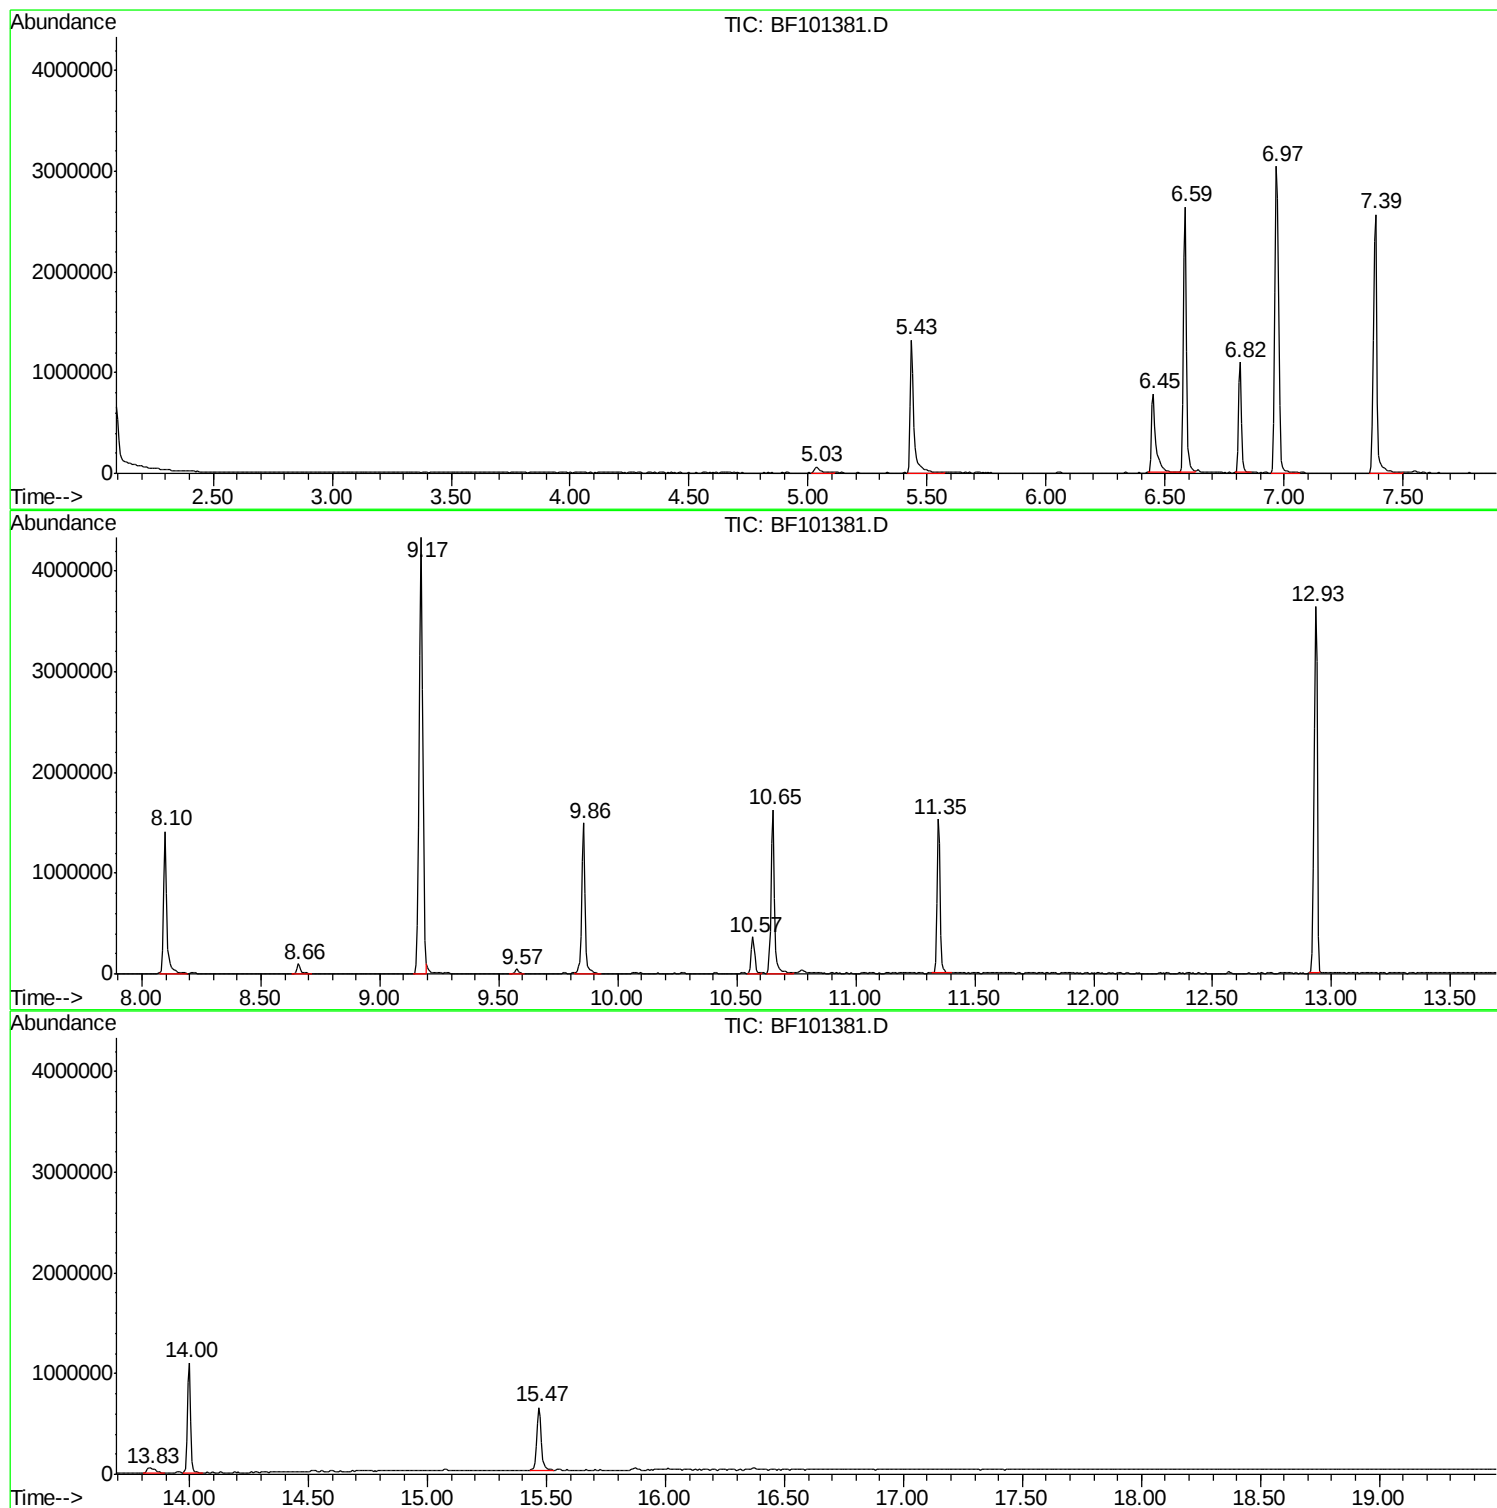

Data_Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF121317\
Data_File : BF101381.D
Acq_On : 13-Dec-2017 23:222
Operator : SJ/JUU
Sample : I6816-088
Misc :
ALS_Vial : 9 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
120717-TIDO-F-D-S

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
