

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF121317\
 Data File : BF101382.D
 Acq On : 13 Dec 2017 23:49
 Operator : SJ/JU
 Sample : I6816-09
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 120717-TIDO-F-U-B

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.039	499	502	515	rBV	44622	68243	1.34%	0.215%
2	5.434	566	569	589	rBV	1449188	1776272	34.86%	5.601%
3	6.451	738	742	761	rBV	904216	1197459	23.50%	3.776%
4	6.586	761	765	772	rBV	3028364	2826643	55.47%	8.913%
5	6.816	800	804	811	rBV	1212356	1066634	20.93%	3.363%
6	6.969	826	830	834	rBV	3338868	3597845	70.60%	11.345%
7	7.386	895	901	904	rBV	2957885	3096612	60.77%	9.764%
8	8.098	1018	1022	1035	rVB	1462216	1441112	28.28%	4.544%
9	8.657	1114	1117	1126	rBV	90258	92919	1.82%	0.293%
10	9.175	1199	1205	1208	rBV	4652183	5095773	100.00%	16.068%
11	9.857	1314	1321	1331	rVB	1510599	1571761	30.84%	4.956%
12	10.569	1438	1442	1448	rVB	289838	249460	4.90%	0.787%
13	10.651	1452	1456	1471	rBV	1814817	1875603	36.81%	5.914%
14	11.345	1570	1574	1583	rBV	1485492	1514413	29.72%	4.775%
15	12.939	1839	1845	1848	rBV	3696961	4135252	81.15%	13.039%
16	13.833	1992	1997	2008	rBV4	50981	135708	2.66%	0.428%
17	13.998	2021	2025	2033	rVB	1141752	1089737	21.39%	3.436%
18	15.468	2268	2275	2285	rBV	639161	882719	17.32%	2.783%


Sum of corrected areas: 31714165

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF121317\
Data File : BF101382.D
Acq On : 13 Dec 2017 23:49
Operator : SJ/JU
Sample : I6816-09
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
120717-TIDO-F-U-B

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

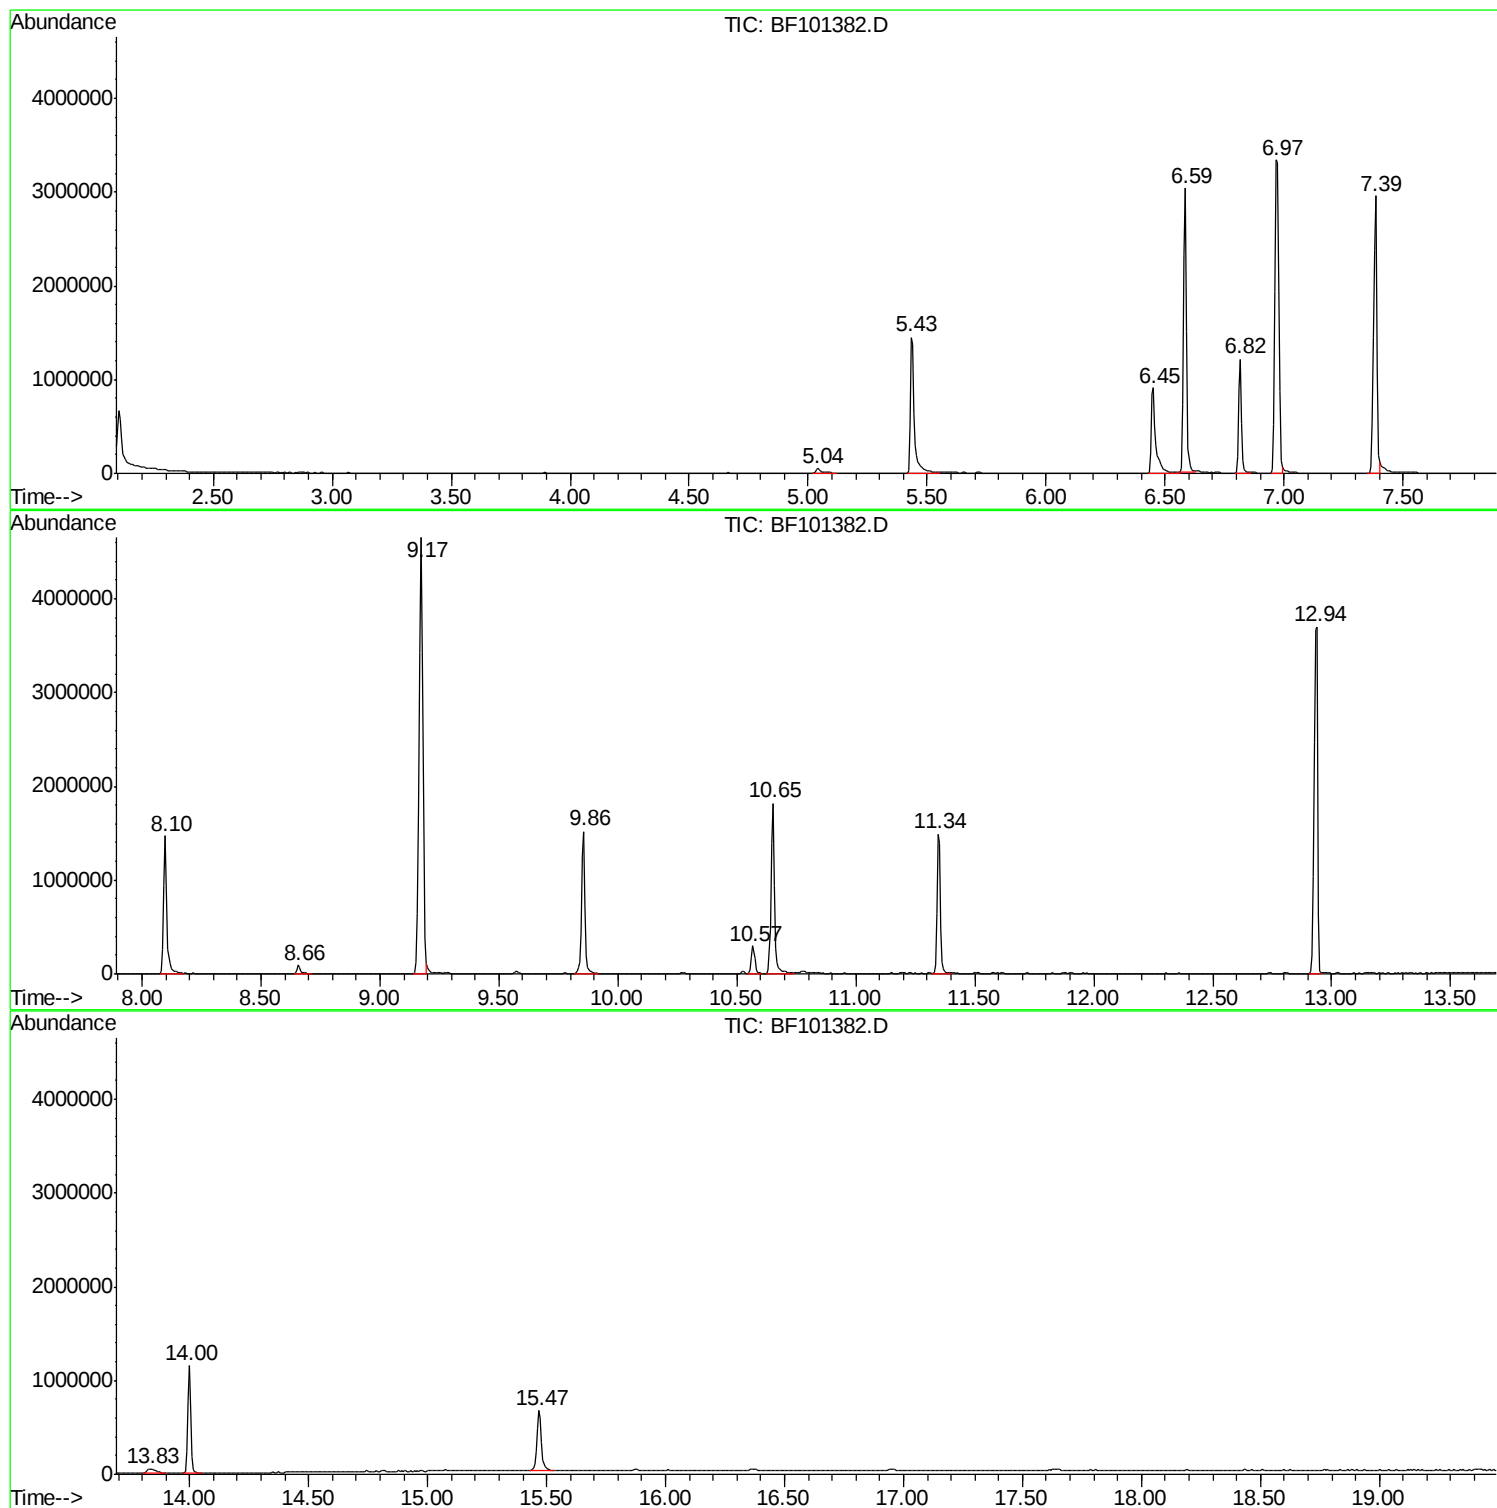

Data_Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF121317\
Data_File : BF101382.D
Acq_On : 13-Dec-2017 23:499
Operator : SJ/JUU
Sample : I6816-099
Misc :
ALS_Vial : 10 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
120717-TIDO-F-U-B

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
