

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF121317\
 Data File : BF101383.D
 Acq On : 14 Dec 2017 00:15
 Operator : SJ/JU
 Sample : I6816-10
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 120717-TIDO-F-U-S

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.034	499	501	513	rBV	46136	79306	1.55%	0.245%
2	5.434	566	569	586	rBV	1531774	1754000	34.30%	5.424%
3	6.451	738	742	761	rBV	945170	1252207	24.49%	3.872%
4	6.587	761	765	772	rBV	3005813	2838413	55.51%	8.777%
5	6.816	800	804	811	rBV	1182474	1074590	21.01%	3.323%
6	6.969	826	830	834	rBV	3372129	3621344	70.82%	11.198%
7	7.387	895	901	904	rBV	2904421	3142336	61.45%	9.717%
8	8.098	1018	1022	1038	rVB	1424164	1435822	28.08%	4.440%
9	8.657	1114	1117	1124	rBV	91175	97784	1.91%	0.302%
10	9.175	1199	1205	1208	rBV	4620751	5113544	100.00%	15.813%
11	9.857	1315	1321	1332	rVB	1526540	1579999	30.90%	4.886%
12	10.569	1438	1442	1448	rBV	312079	266511	5.21%	0.824%
13	10.651	1452	1456	1470	rBV	1905584	1923705	37.62%	5.949%
14	11.345	1570	1574	1583	rBV	1557878	1503433	29.40%	4.649%
15	12.933	1839	1844	1848	rBV	3706313	4265937	83.42%	13.192%
16	13.839	1992	1998	2007	rBV5	39432	103110	2.02%	0.319%
17	13.998	2021	2025	2033	rVB	1146848	1085534	21.23%	3.357%
18	15.468	2267	2275	2285	rBV	672608	915662	17.91%	2.832%
19	15.874	2339	2344	2349	rVB2	46266	64808	1.27%	0.200%
20	16.368	2423	2428	2435	rBV2	48596	86514	1.69%	0.268%
21	16.951	2522	2527	2533	rVB2	34828	69124	1.35%	0.214%
22	17.639	2640	2644	2654	rVB3	26971	64093	1.25%	0.198%


Sum of corrected areas: 32337776

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF121317\
Data File : BF101383.D
Acq On : 14 Dec 2017 00:15
Operator : SJ/JU
Sample : I6816-10
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
120717-TIDO-F-U-S

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

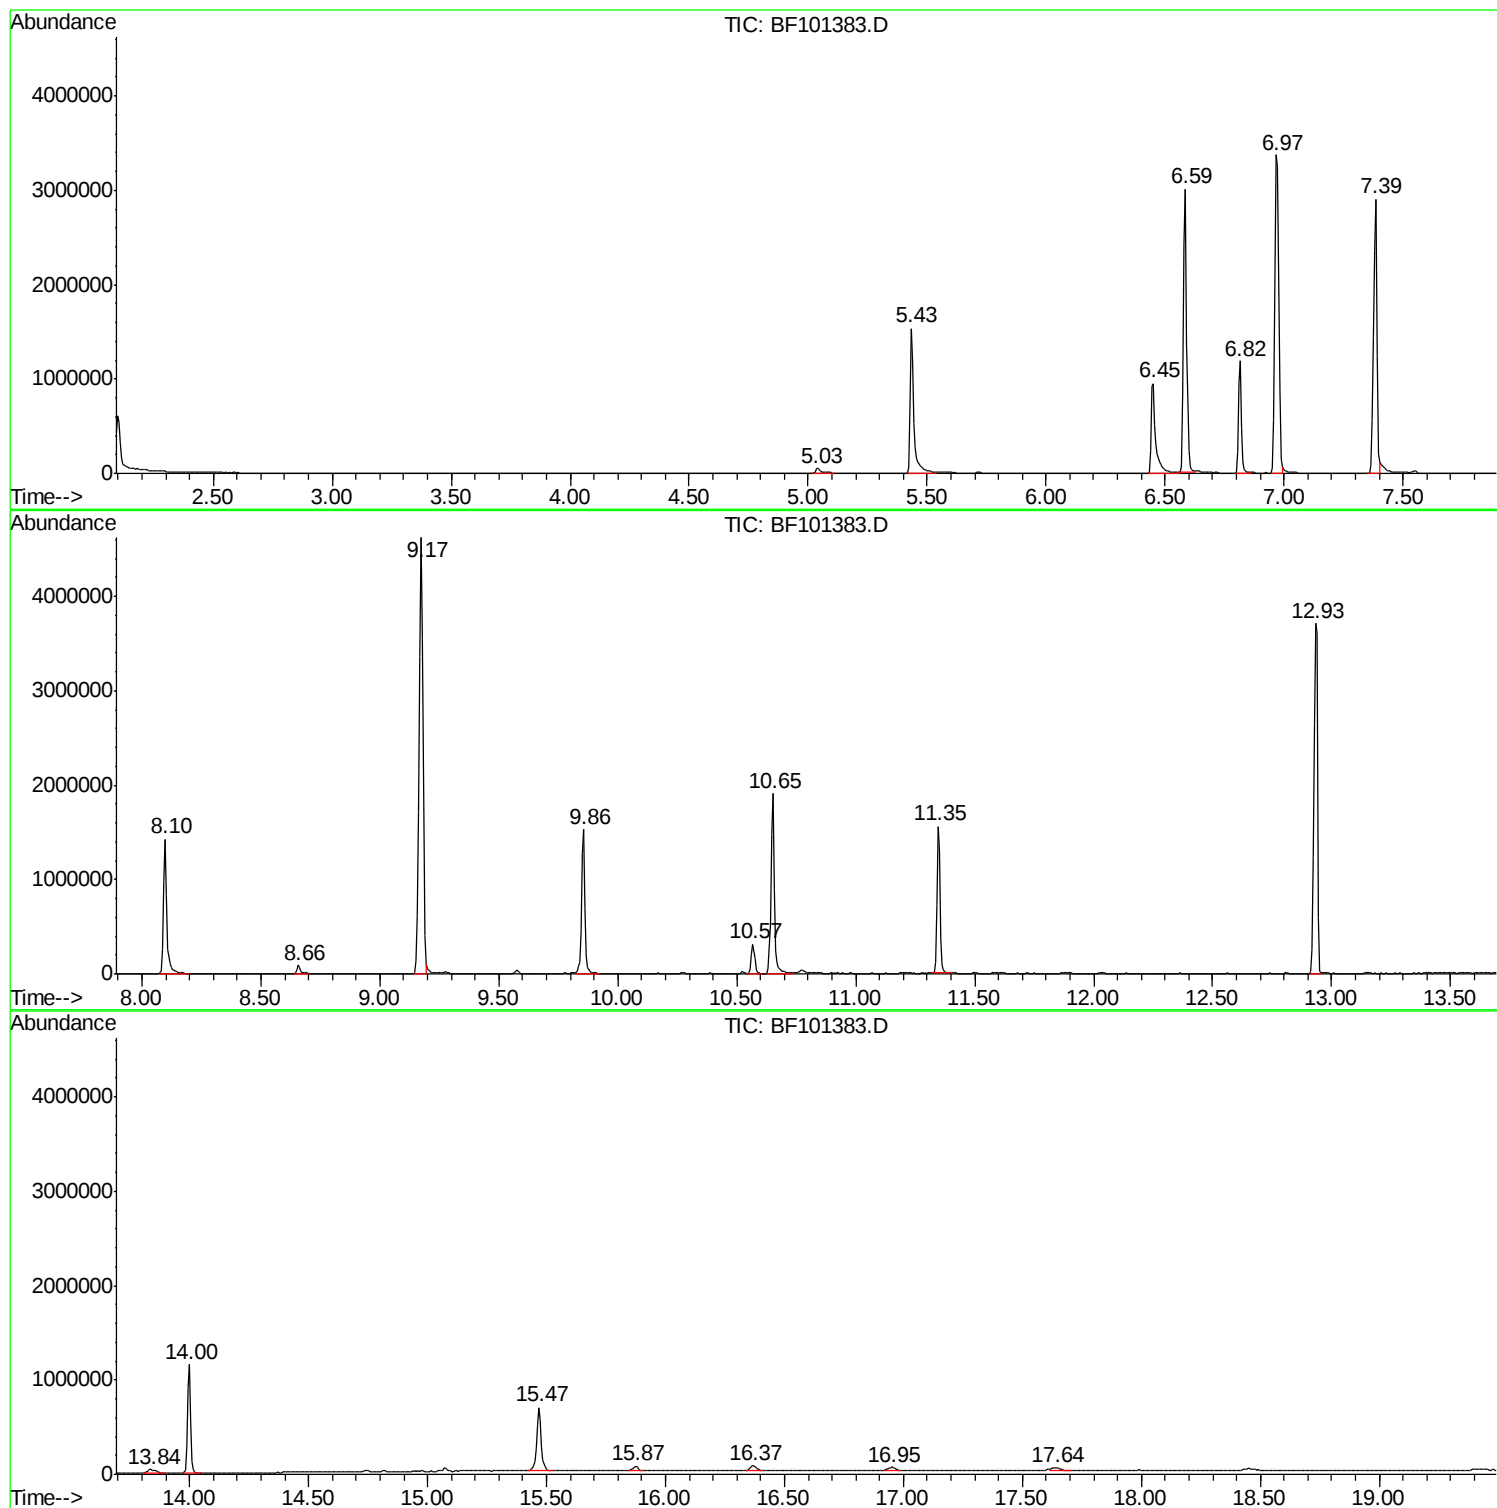

Data_Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF121317\
Data_File : BF101383.D
Acq_On : 14 Dec 2017 00:155
Operator : SJ/JUU
Sample : I6816-100
Misc :
ALS_Vial : 11 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
120717-TIDO-F-U-S

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
