

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF121317\
 Data File : BF101384.D
 Acq On : 14 Dec 2017 00:42
 Operator : SJ/JU
 Sample : I6816-11
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 120717-FOPI-F-D-B

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.028	498	500	514	rBV	103472	153064	3.29%	0.511%
2	5.434	566	569	590	rBV	1339772	1568991	33.72%	5.234%
3	6.451	738	742	755	rBV	735081	1049388	22.56%	3.501%
4	6.587	761	765	772	rBV	2679716	2611517	56.13%	8.711%
5	6.816	800	804	812	rBV	1097836	1037051	22.29%	3.459%
6	6.969	826	830	840	rBV	3225963	3343855	71.87%	11.154%
7	7.387	895	901	918	rBV	2652916	2982087	64.10%	9.948%
8	8.098	1018	1022	1036	rVB	1365858	1378101	29.62%	4.597%
9	8.657	1113	1117	1126	rBV	97434	102774	2.21%	0.343%
10	9.175	1199	1205	1208	rBV	4488668	4652344	100.00%	15.519%
11	9.575	1269	1273	1279	rBV	43863	47727	1.03%	0.159%
12	9.857	1313	1321	1334	rVB	1481823	1519930	32.67%	5.070%
13	10.569	1438	1442	1448	rVB	328428	291392	6.26%	0.972%
14	10.651	1452	1456	1471	rBV	1634732	1764086	37.92%	5.885%
15	11.345	1570	1574	1583	rBV	1507939	1464791	31.49%	4.886%
16	12.933	1839	1844	1847	rBV	3620933	3949520	84.89%	13.175%
17	13.839	1991	1998	2007	rBV6	35703	99986	2.15%	0.334%
18	13.998	2021	2025	2034	rBV	1118675	1082639	23.27%	3.611%
19	15.468	2269	2275	2285	rBV	646083	878781	18.89%	2.931%


Sum of corrected areas: 29978024

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF121317\
Data File : BF101384.D
Acq On : 14 Dec 2017 00:42
Operator : SJ/JU
Sample : I6816-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
120717-FOPI-F-D-B

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

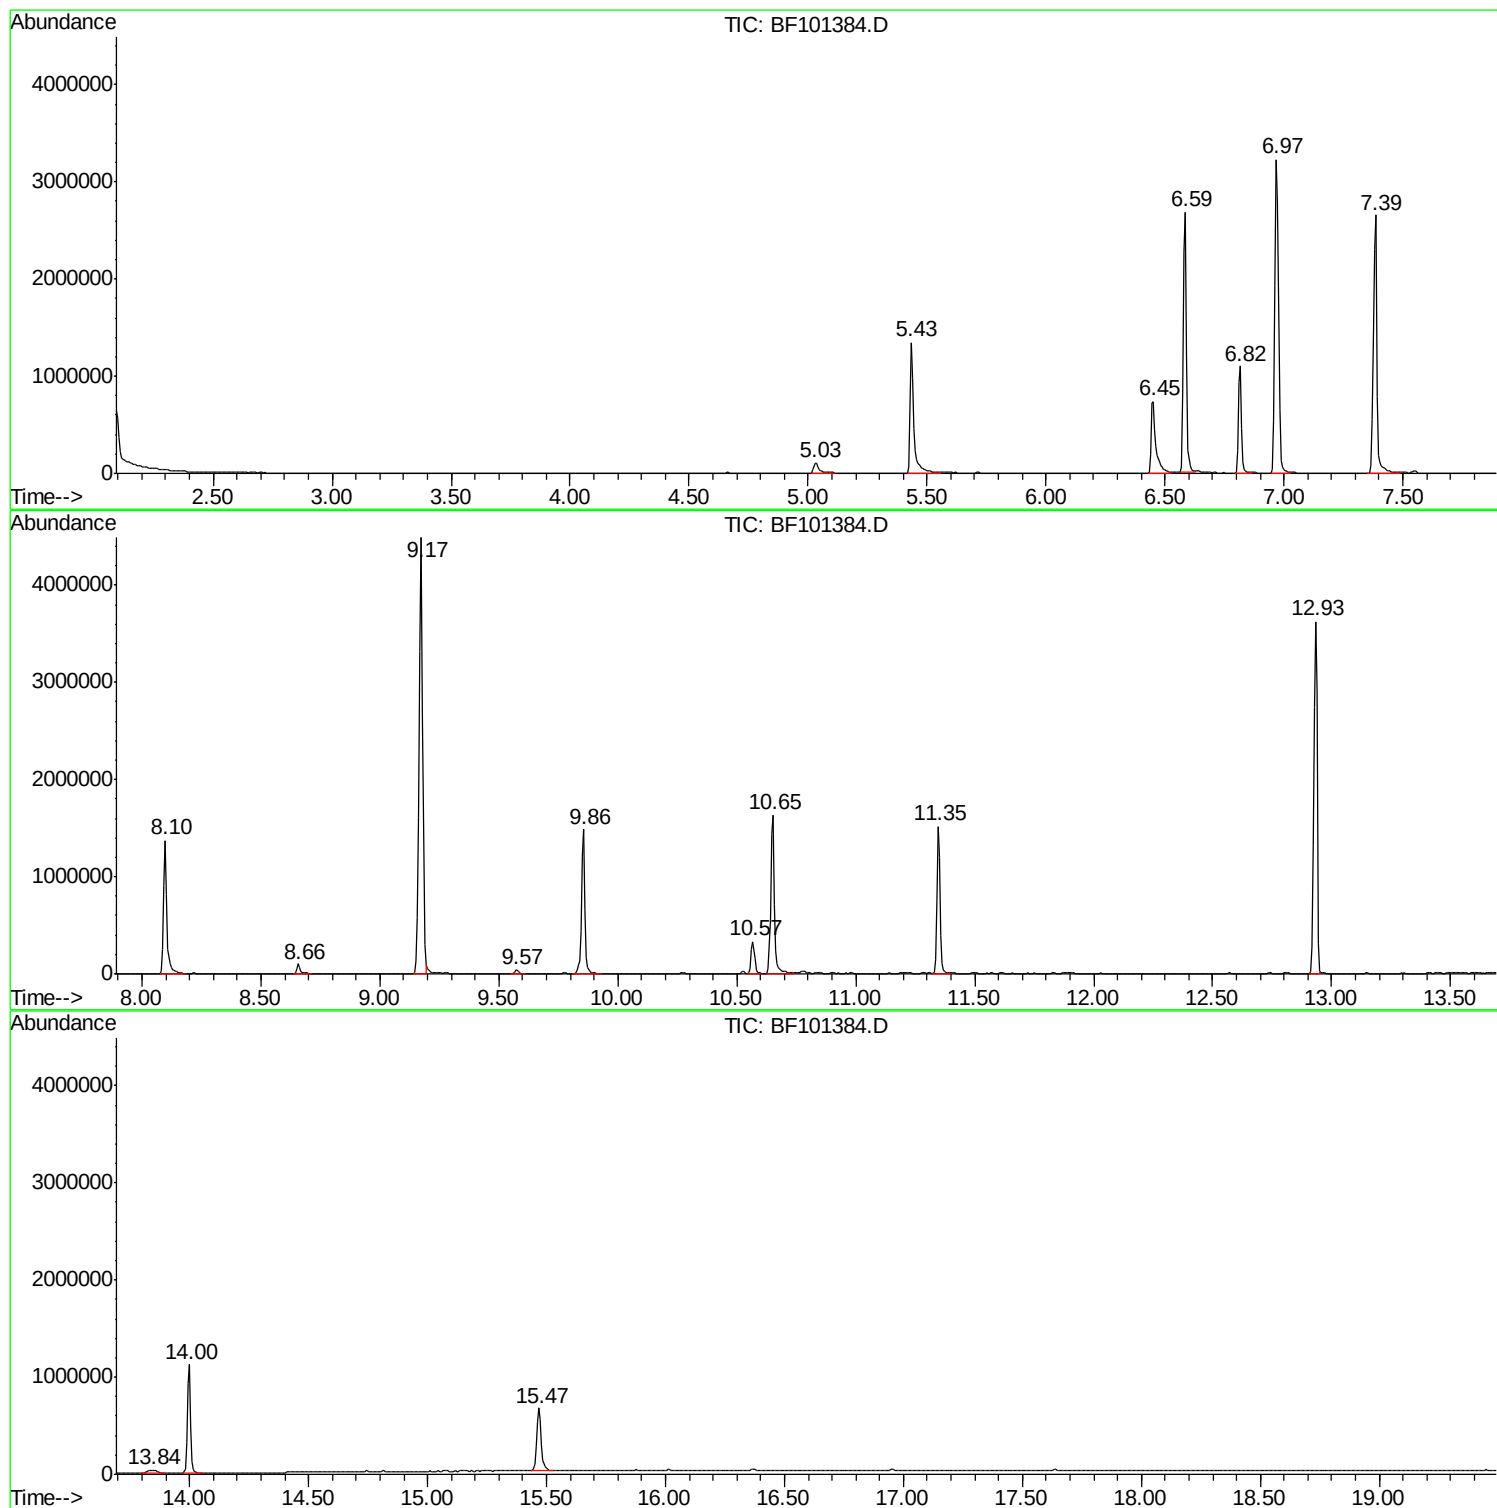

Data_Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF121317\
Data_File : BF101384.D
Acq_On : 14 Dec 2017 00:422
Operator : SJ/JUU
Sample : I6816-111
Misc :
ALS_Vial : 12 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
120717-FOPI-F-D-B

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
