

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF121317\
 Data File : BF101385.D
 Acq On : 14 Dec 2017 1:09
 Operator : SJ/JU
 Sample : I6816-12
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 120717-FOPI-F-D-S

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.028	497	500	516	rBV	106703	152691	3.19%	0.503%
2	5.434	566	569	589	rBV	1360938	1552561	32.44%	5.112%
3	6.451	738	742	761	rBV	742394	1031171	21.55%	3.395%
4	6.587	761	765	771	rBV	2754942	2621783	54.79%	8.633%
5	6.816	800	804	812	rBV	1128165	1024497	21.41%	3.373%
6	6.969	826	830	844	rBV	3252267	3509634	73.34%	11.556%
7	7.387	895	901	922	rBV	2806200	3069174	64.14%	10.106%
8	8.098	1018	1022	1039	rVB	1369936	1382420	28.89%	4.552%
9	8.657	1113	1117	1127	rBV	97453	104329	2.18%	0.344%
10	9.175	1199	1205	1208	rBV	4571882	4785290	100.00%	15.757%
11	9.857	1314	1321	1336	rVB	1414875	1524693	31.86%	5.020%
12	10.569	1438	1442	1450	rBV	328024	295874	6.18%	0.974%
13	10.651	1452	1456	1470	rBV	1657246	1793939	37.49%	5.907%
14	11.345	1570	1574	1583	rBV	1486074	1456655	30.44%	4.796%
15	12.933	1839	1844	1848	rBV	3652862	4011236	83.82%	13.208%
16	13.839	1992	1998	2003	rBV6	29641	74426	1.56%	0.245%
17	13.998	2021	2025	2032	rBV	1069077	1023075	21.38%	3.369%
18	15.468	2267	2275	2282	rBV	603469	848037	17.72%	2.792%
19	16.368	2423	2428	2433	rVB3	33725	56726	1.19%	0.187%
20	16.951	2522	2527	2535	rVB3	24837	51312	1.07%	0.169%


Sum of corrected areas: 30369523

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF121317\
Data File : BF101385.D
Acq On : 14 Dec 2017 1:09
Operator : SJ/JU
Sample : I6816-12
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
120717-FOPI-F-D-S

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

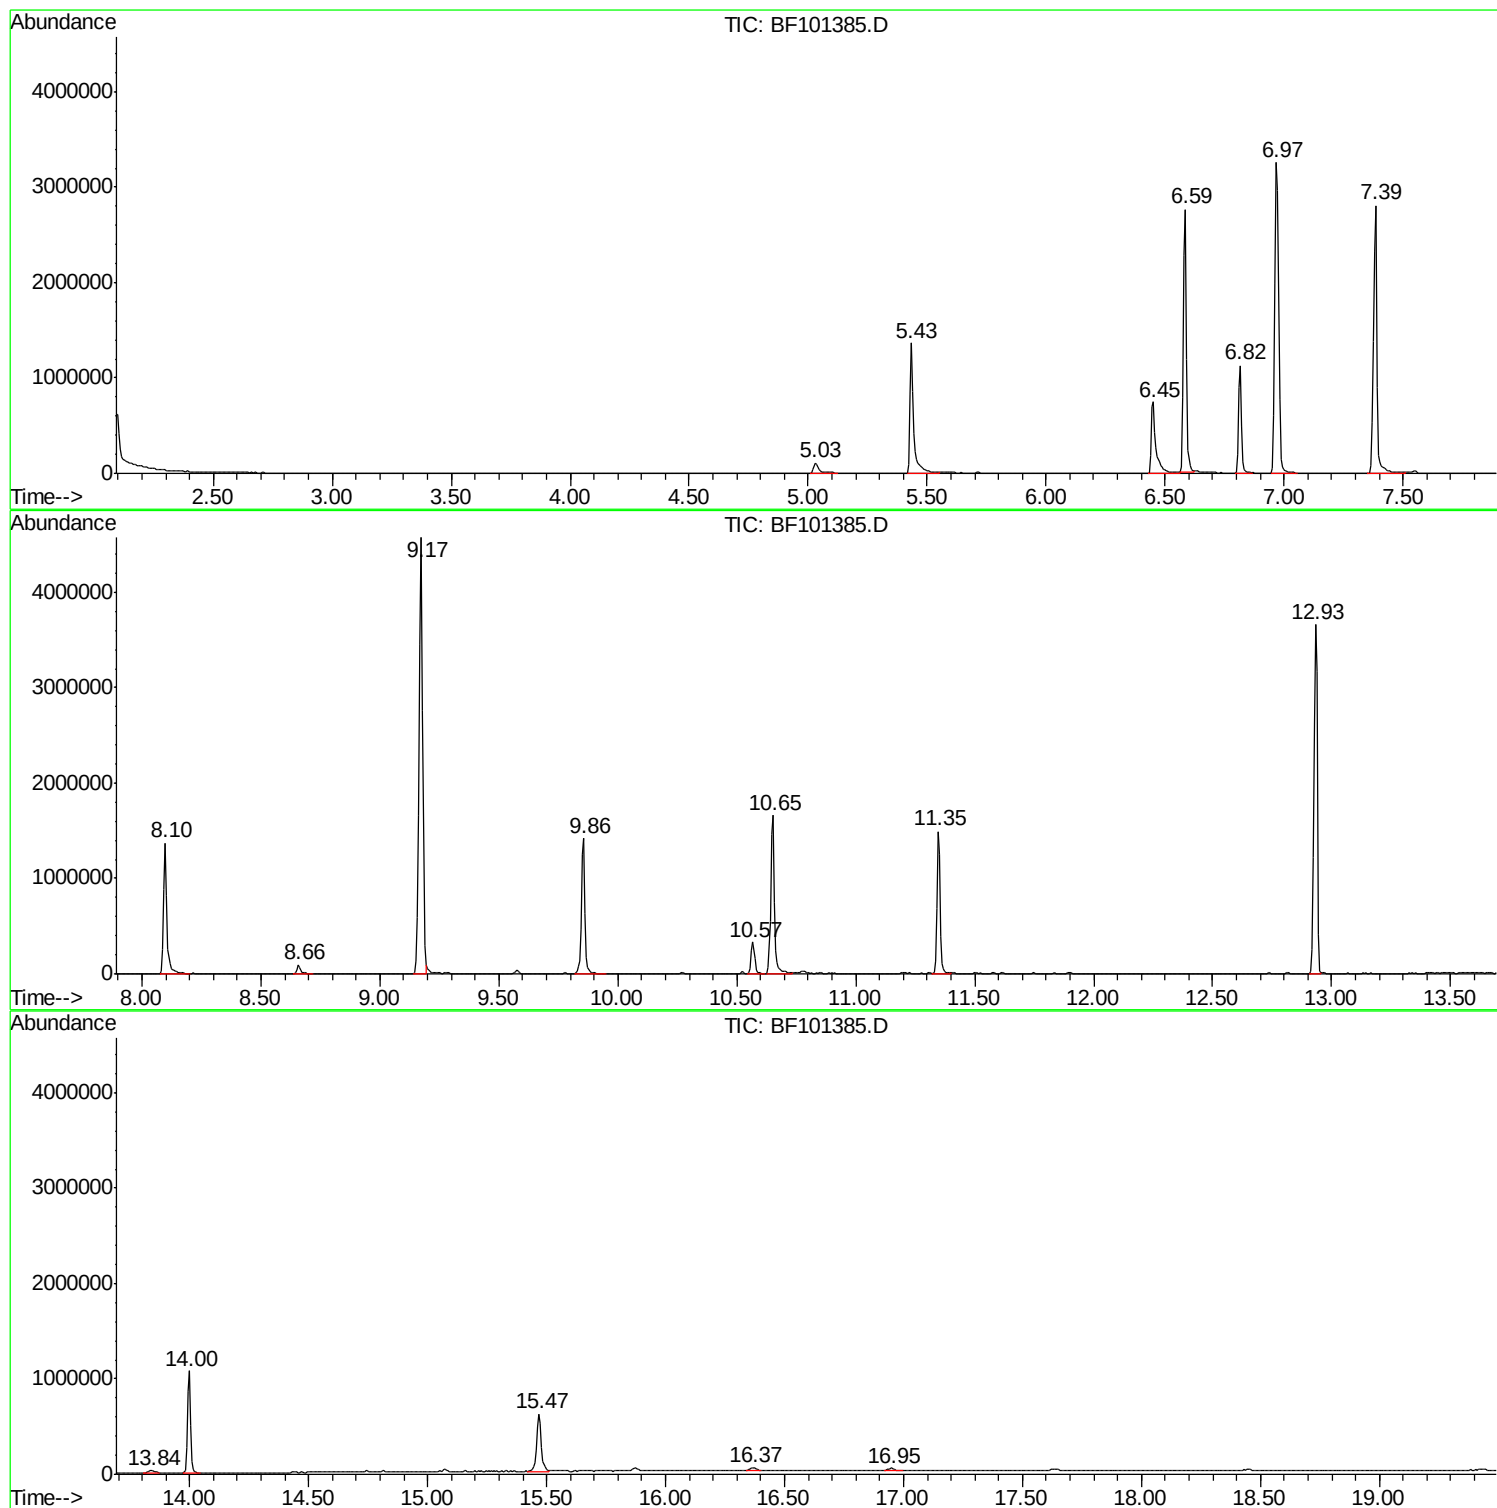

Data_Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF121317\
Data_File : BF101385.D
Acq_On : 14 Dec 2017 1:099
Operator : SJ/JUU
Sample : I6816-122
Misc :
ALS_Vial : 13 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
120717-FOPI-F-D-S

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
