


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA F\Data\BF121317\
 Data File : BF101373.D
 Acq On : 13 Dec 2017 19:39
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 08 18:17:31 2017

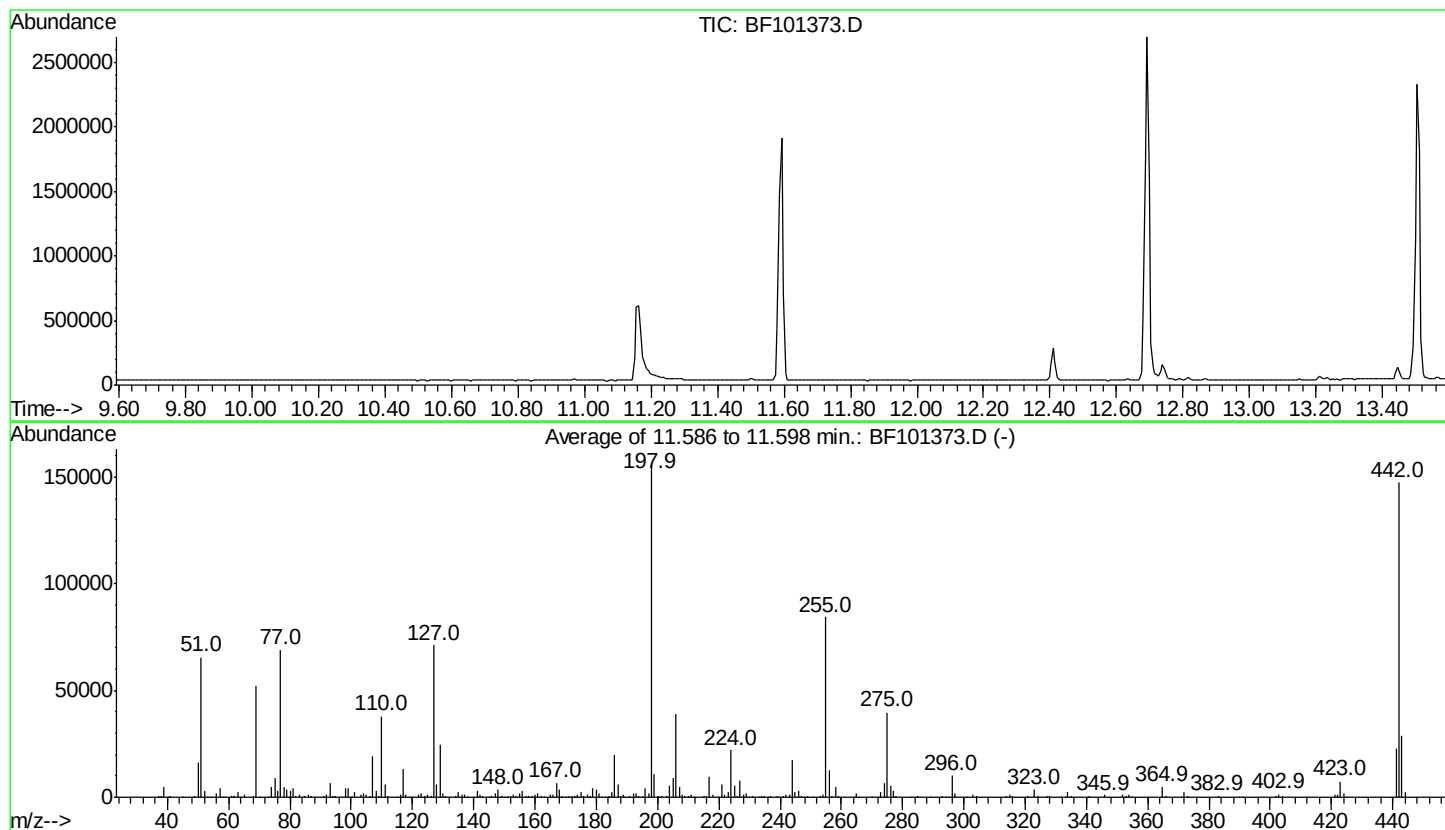

AutoFind: Scans 1615, 1616, 1617; Background Corrected with Scan 1609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.2	65646	PASS
68	69	0.00	2	1.6	859	PASS
69	198	0.00	100	33.6	52234	PASS
70	69	0.00	2	0.2	102	PASS
127	198	10	80	45.8	71264	PASS
197	198	0.00	2	1.0	1595	PASS
198	198	100	100	100.0	155448	PASS
199	198	5	9	7.0	10848	PASS
275	198	10	60	25.5	39701	PASS
365	198	1	100	3.3	5109	PASS
441	443	0.01	100	78.6	22781	PASS
442	198	50	100	94.9	147458	PASS
443	442	15	24	19.7	28986	PASS