
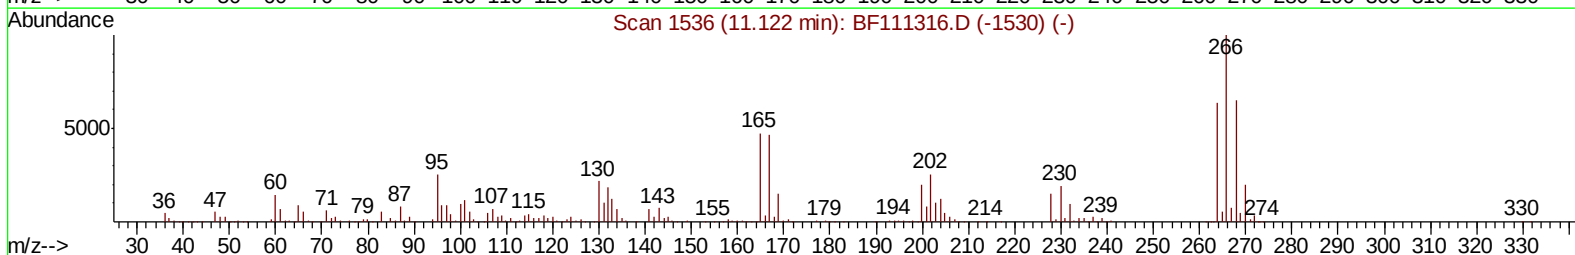
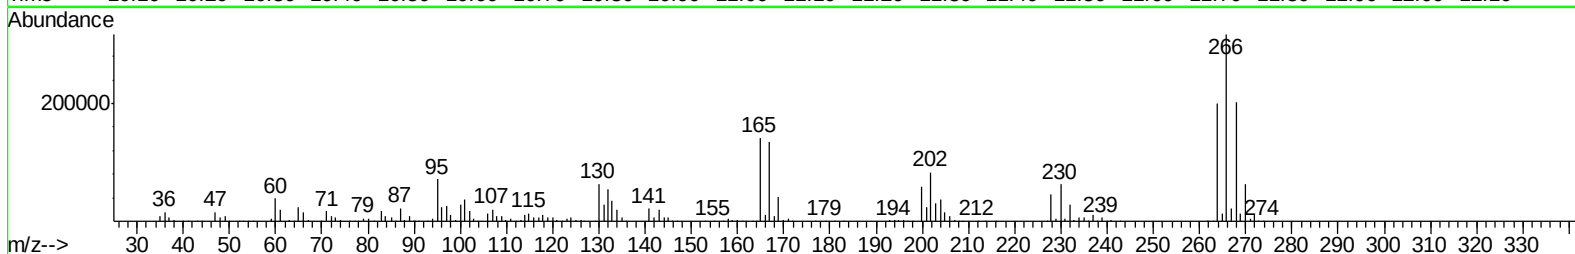


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121318\
 Data File : BF111358.D
 Acq On : 13 Dec 2018 9:24
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 14 08:23:13 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF121218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 12 13:16:52 2018
 Response via : Initial Calibration

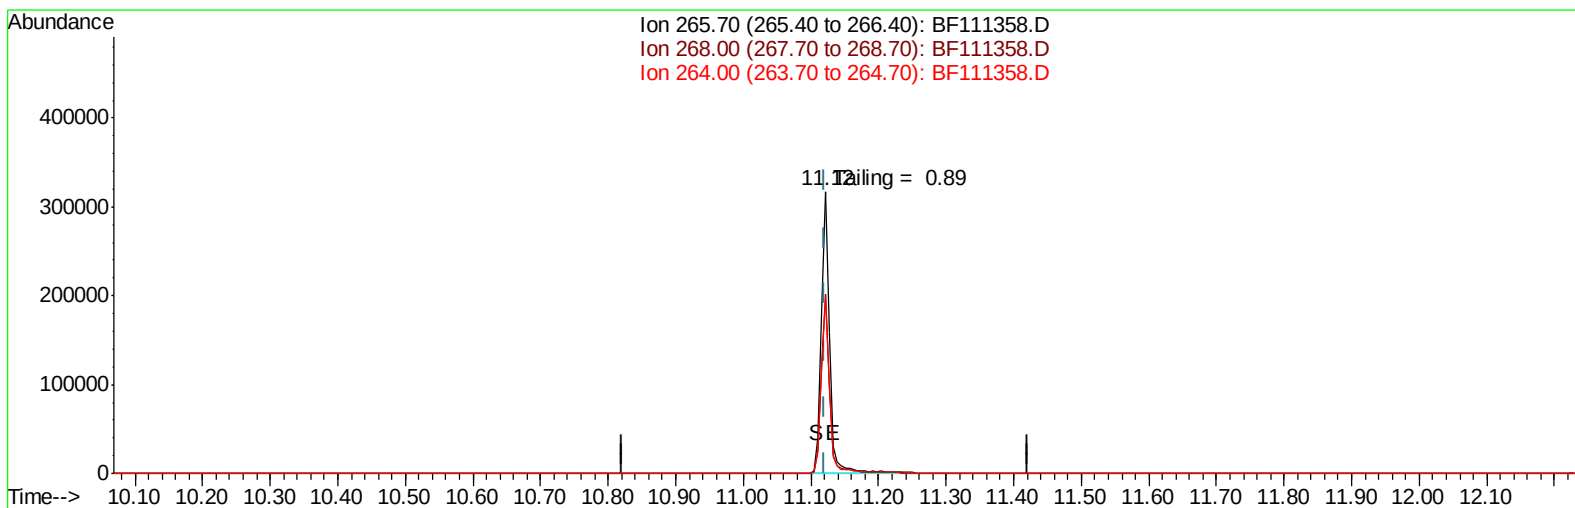

TIC: BF111358.D

(70) Pentachlorophenol (C)




11.122min (+0.000) 24269.92ng

response 282339

Ion	Exp%	Act%
265.70	100	100
268.00	59.90	63.46
264.00	61.40	62.87
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121318\
Data File : BF111358.D
Acq On : 13 Dec 2018 9:24
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 14 08:23:13 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF121218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 13:16:52 2018
Response via : Initial Calibration

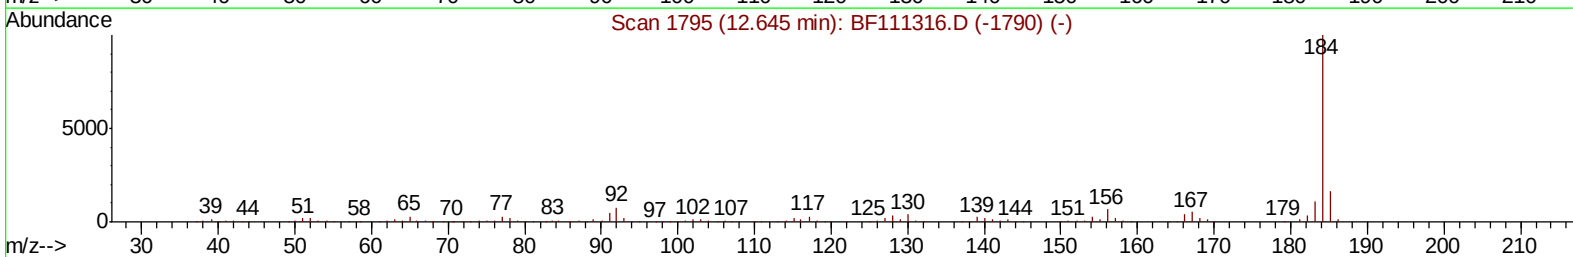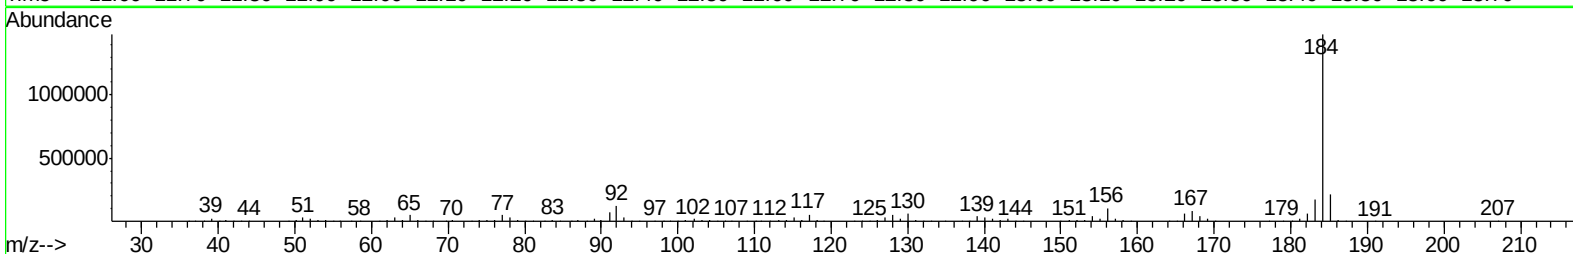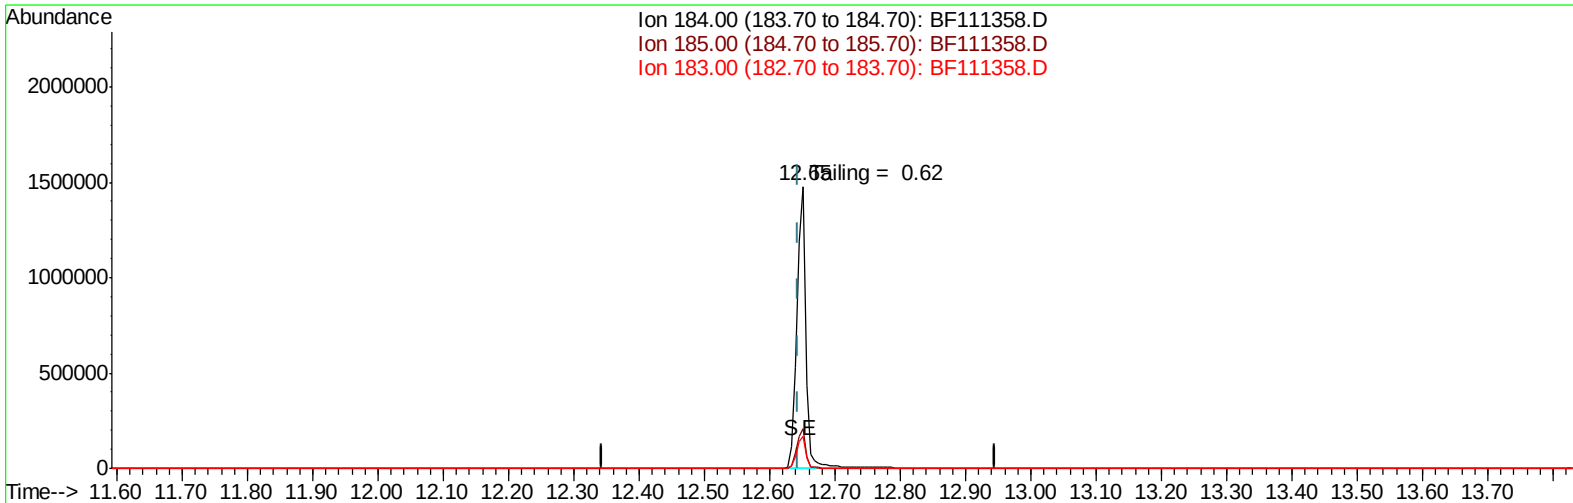

TIC: BF111358.D

(77) Benzidine

12.651min (+0.006) 70067.14ng

response 1442605

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	14.27
183.00	11.60	11.55
0.00	0.00	0.00