
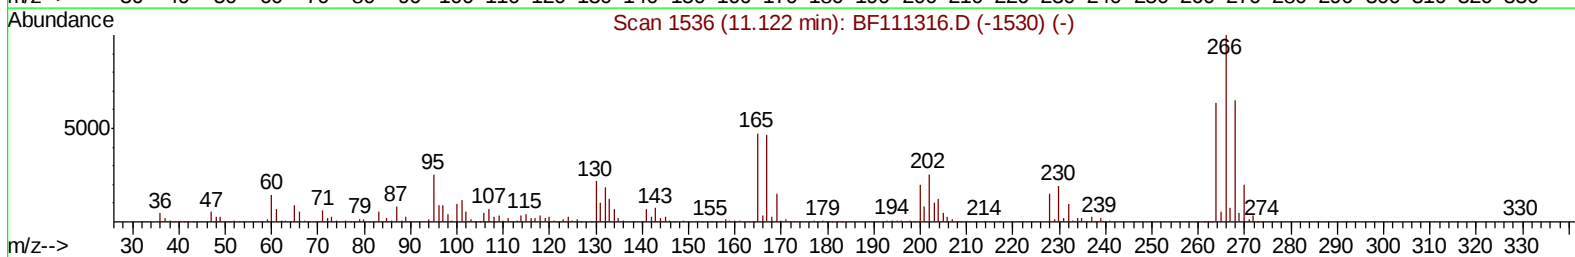
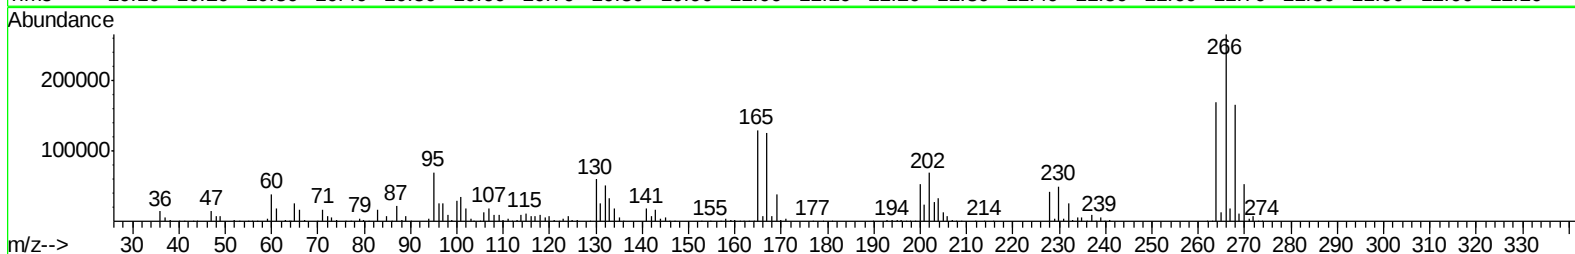


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121318\
Data File : BF111371.D
Acq On : 13 Dec 2018 15:52
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 14 08:25:30 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF121218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 13:16:52 2018
Response via : Initial Calibration

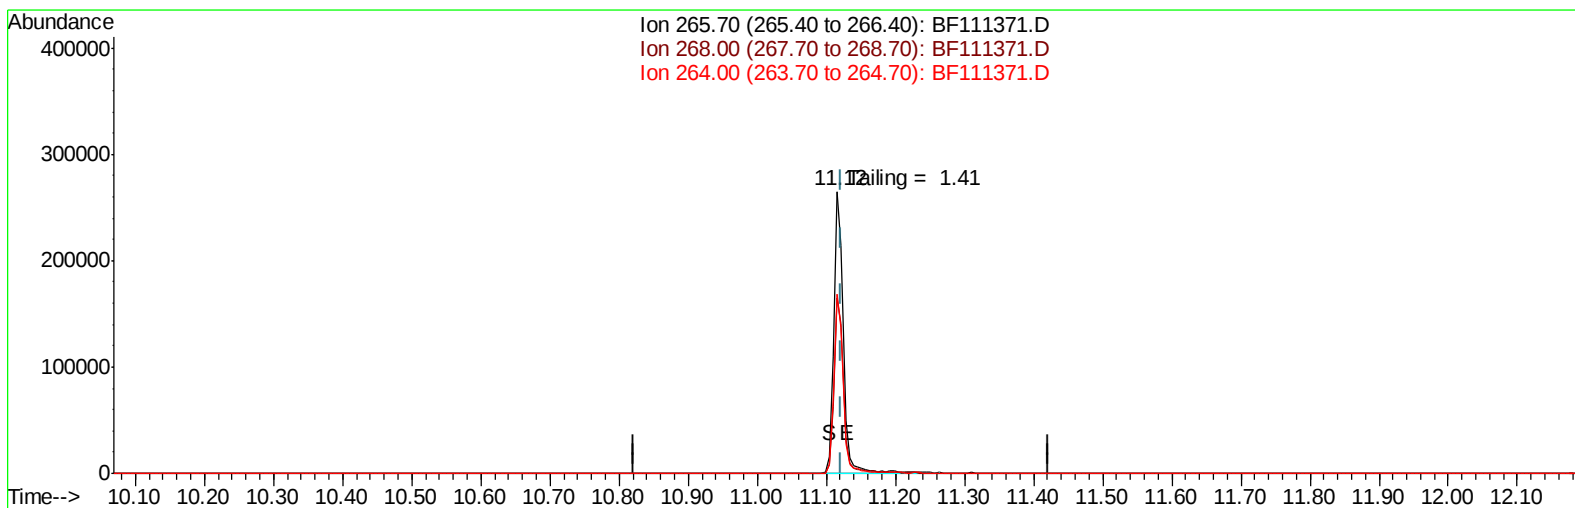

TIC: BF111371.D

(70) Pentachlorophenol (C)




11.116min (-0.006) 28359.06ng

response 247486

Ion	Exp%	Act%
265.70	100	100
268.00	59.90	62.29
264.00	61.40	63.48
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121318\
Data File : BF111371.D
Acq On : 13 Dec 2018 15:52
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 14 08:25:30 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF121218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 13:16:52 2018
Response via : Initial Calibration

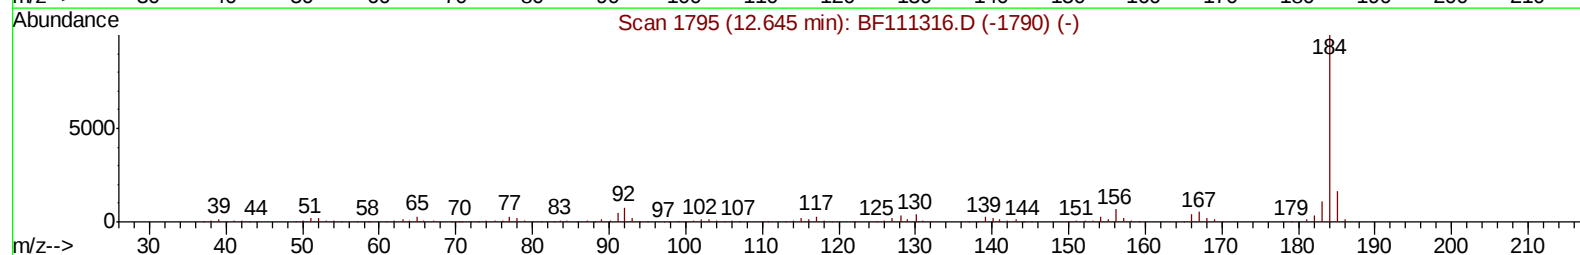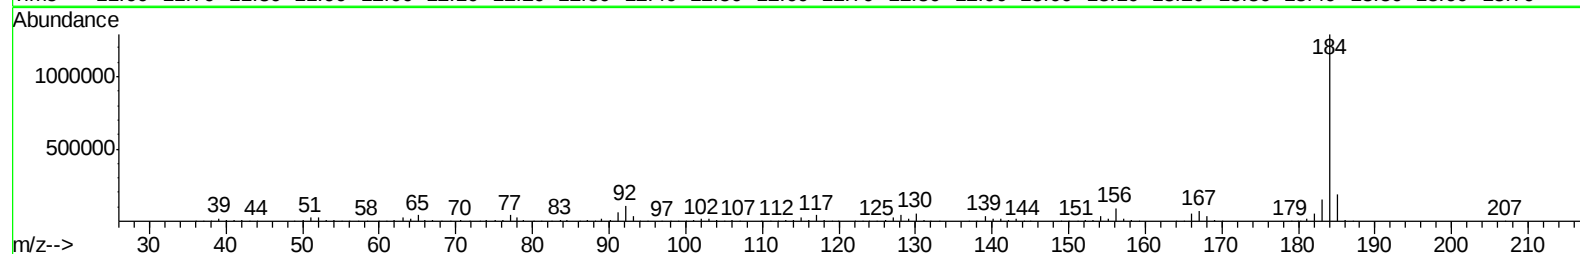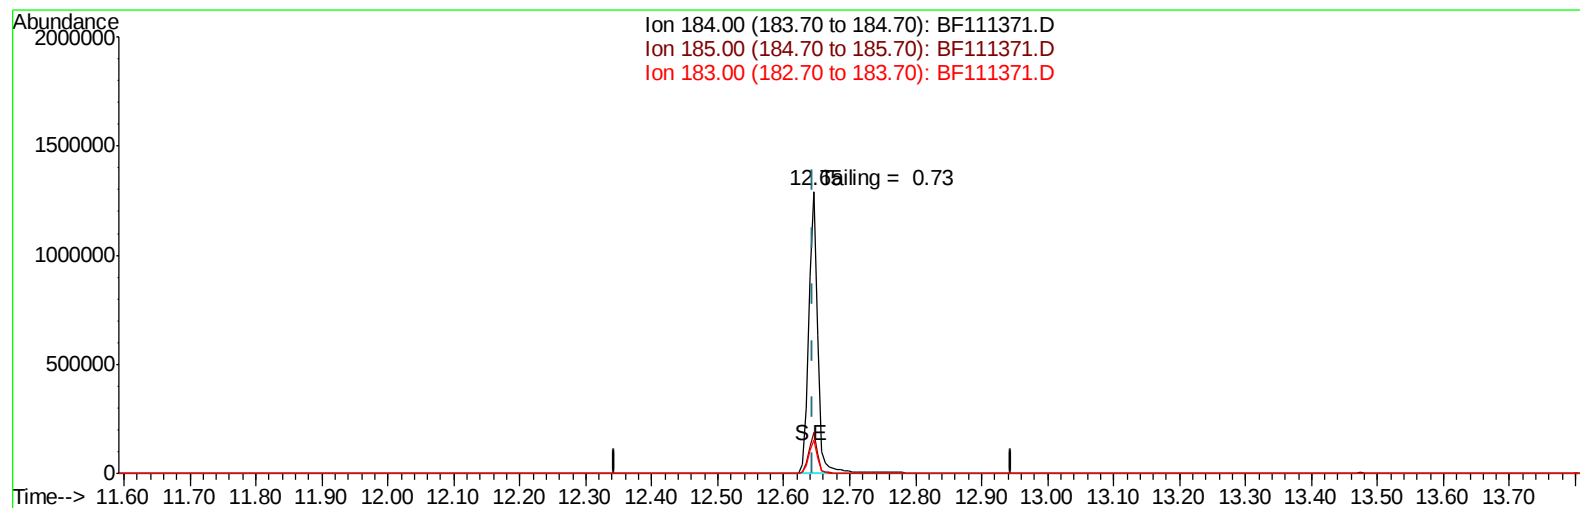

TIC: BF111371.D

(77) Benzidine

12.645min (+0.000) 98602.02ng

response 1237416

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	14.60
183.00	11.60	11.95
0.00	0.00	0.00