


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121318\
 Data File : BF111358.D
 Acq On : 13 Dec 2018 9:24
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF121218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 12 13:16:52 2018

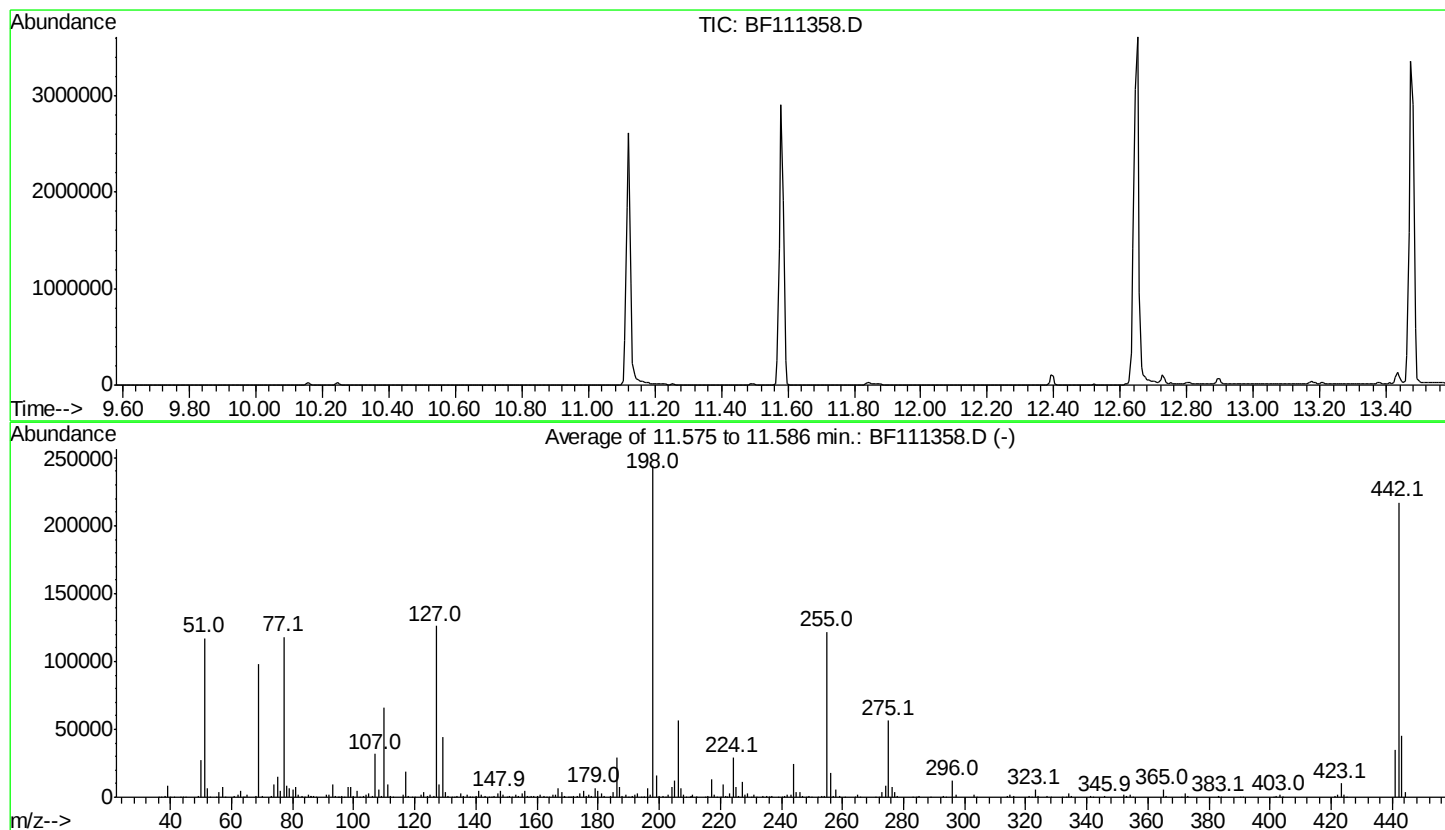

AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.9	116930	PASS
68	69	0.00	2	1.5	1438	PASS
69	198	0.00	100	40.1	98005	PASS
70	69	0.00	2	0.6	591	PASS
127	198	10	80	51.7	126309	PASS
197	198	0.00	2	0.8	1853	PASS
198	198	100	100	100.0	244245	PASS
199	198	5	9	6.7	16280	PASS
275	198	10	60	23.1	56322	PASS
365	198	1	100	2.3	5644	PASS
441	198	0.01	100	14.2	34756	PASS
442	198	50	100	88.9	217013	PASS
443	442	15	24	20.8	45194	PASS