


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121318\
 Data File : BF111398.D
 Acq On : 14 Dec 2018 4:43
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF121218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 12 13:16:52 2018

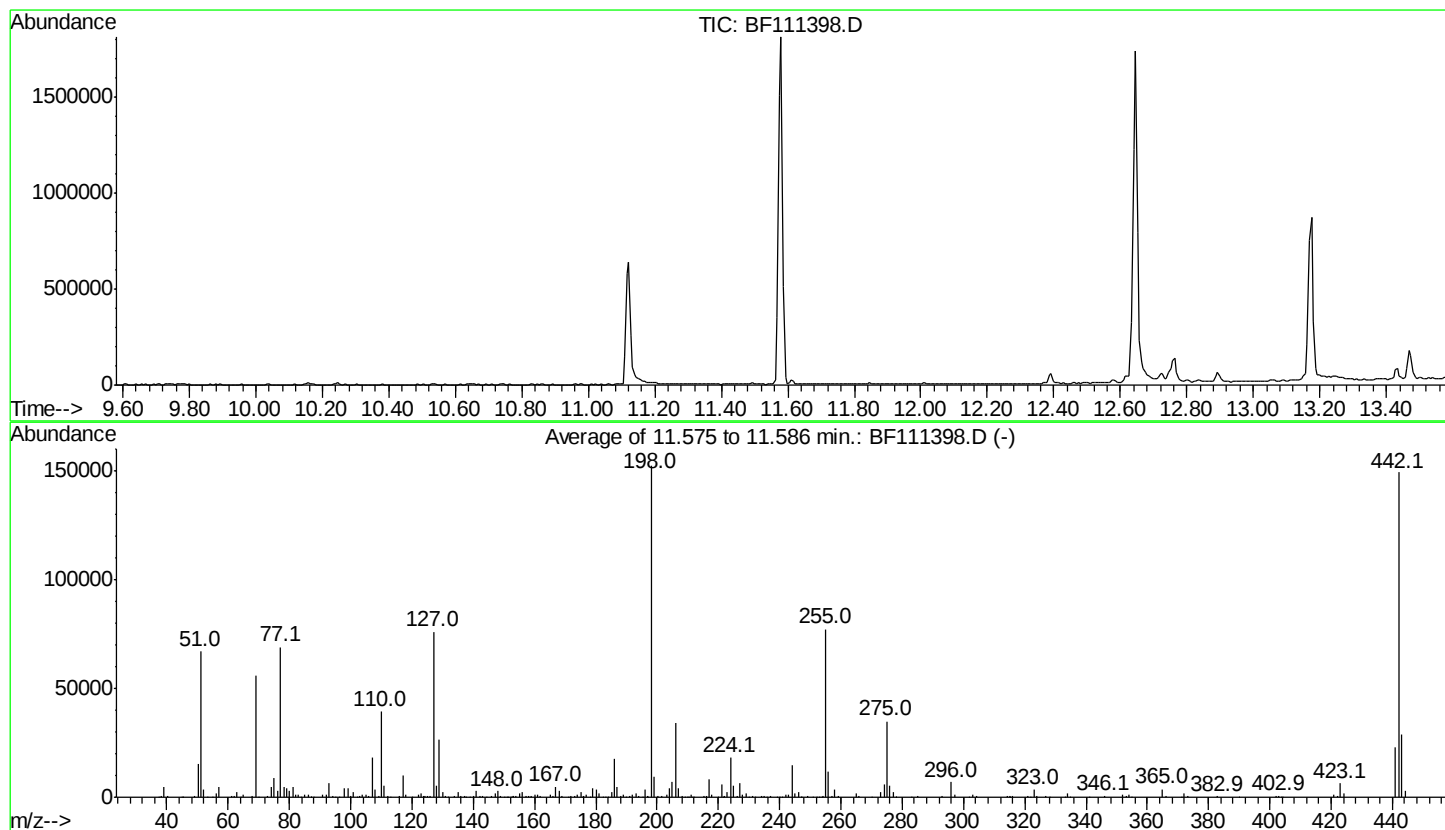

AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.9	66973	PASS
68	69	0.00	2	1.5	840	PASS
69	198	0.00	100	36.6	55857	PASS
70	69	0.00	2	0.5	258	PASS
127	198	10	80	49.9	76106	PASS
197	198	0.00	2	0.5	818	PASS
198	198	100	100	100.0	152592	PASS
199	198	5	9	6.1	9263	PASS
275	198	10	60	22.9	34893	PASS
365	198	1	100	2.5	3807	PASS
441	198	0.01	100	15.2	23160	PASS
442	198	50	100	98.0	149600	PASS
443	442	15	24	19.3	28832	PASS