
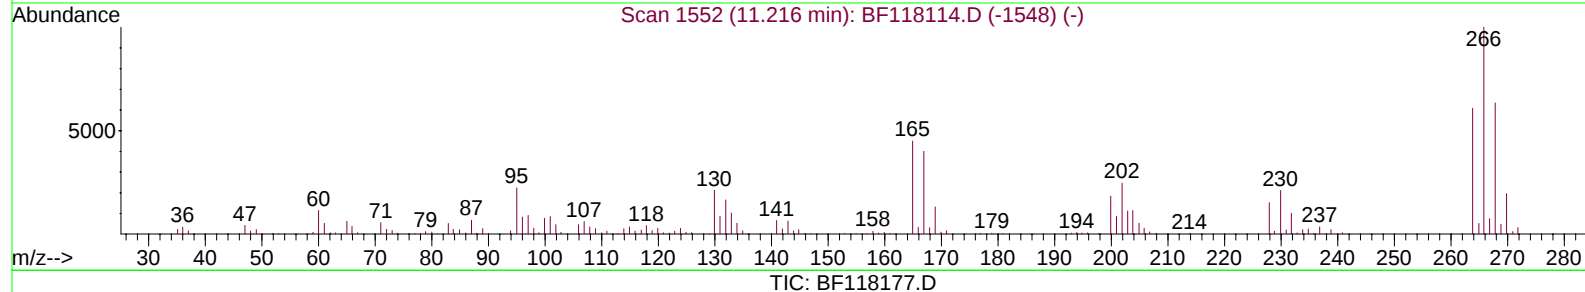
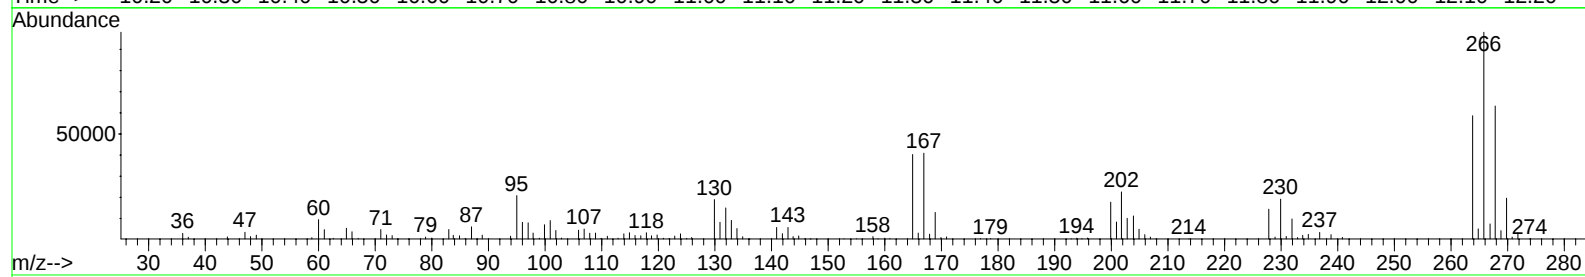


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF121319\
 Data File : BF118177.D
 Acq On : 13 Dec 2019 10:14
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 13 17:58:49 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF120619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 06 17:34:43 2019
 Response via : Initial Calibration

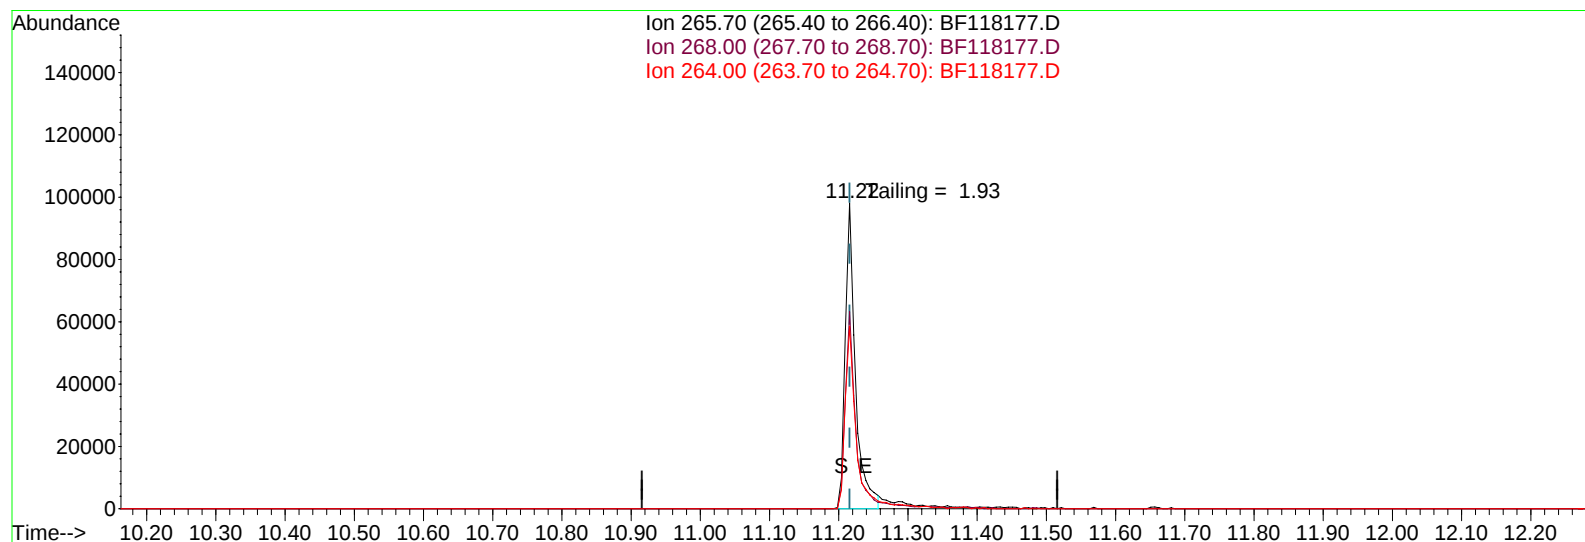

(70) Pentachlorophenol (C)




11.216min (-0.000) 7677.77ng

response 104059

Ion	Exp%	Act%
265.70	100	100
268.00	63.40	64.47
264.00	60.90	59.71
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF121319\
 Data File : BF118177.D
 Acq On : 13 Dec 2019 10:14
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 13 17:58:49 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF120619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 06 17:34:43 2019
 Response via : Initial Calibration

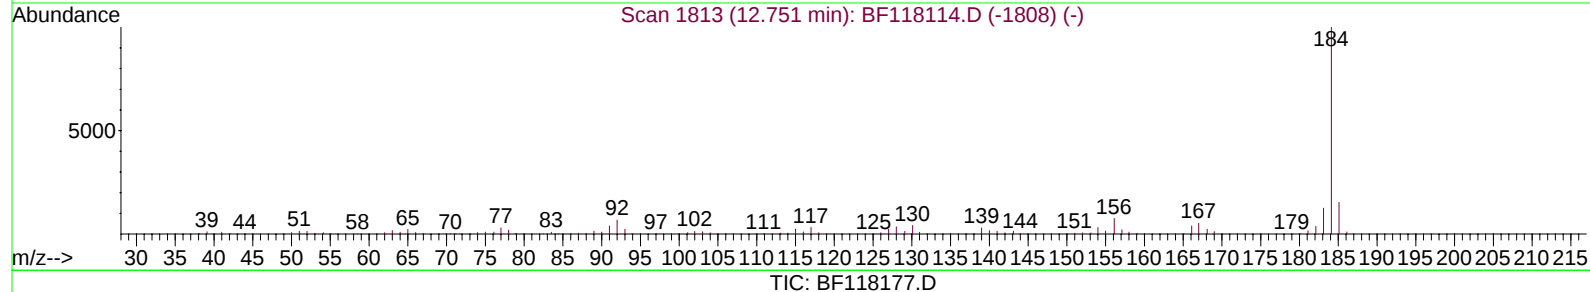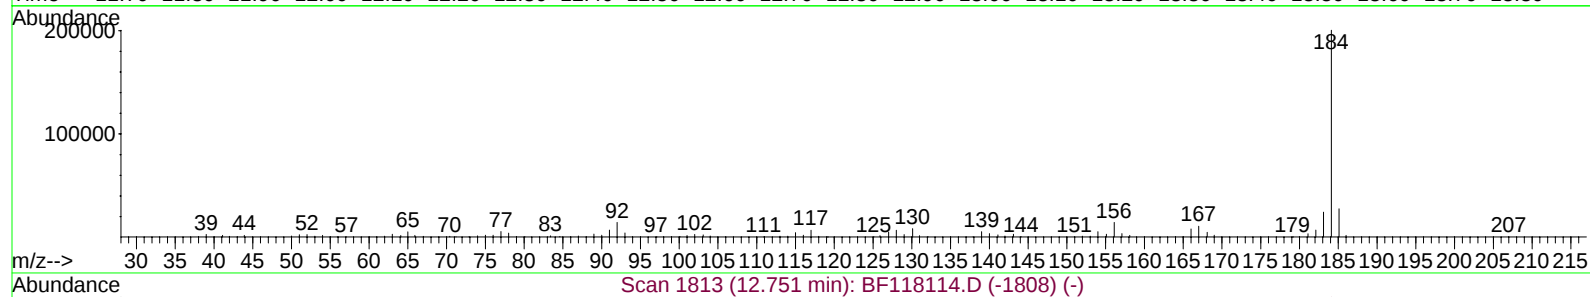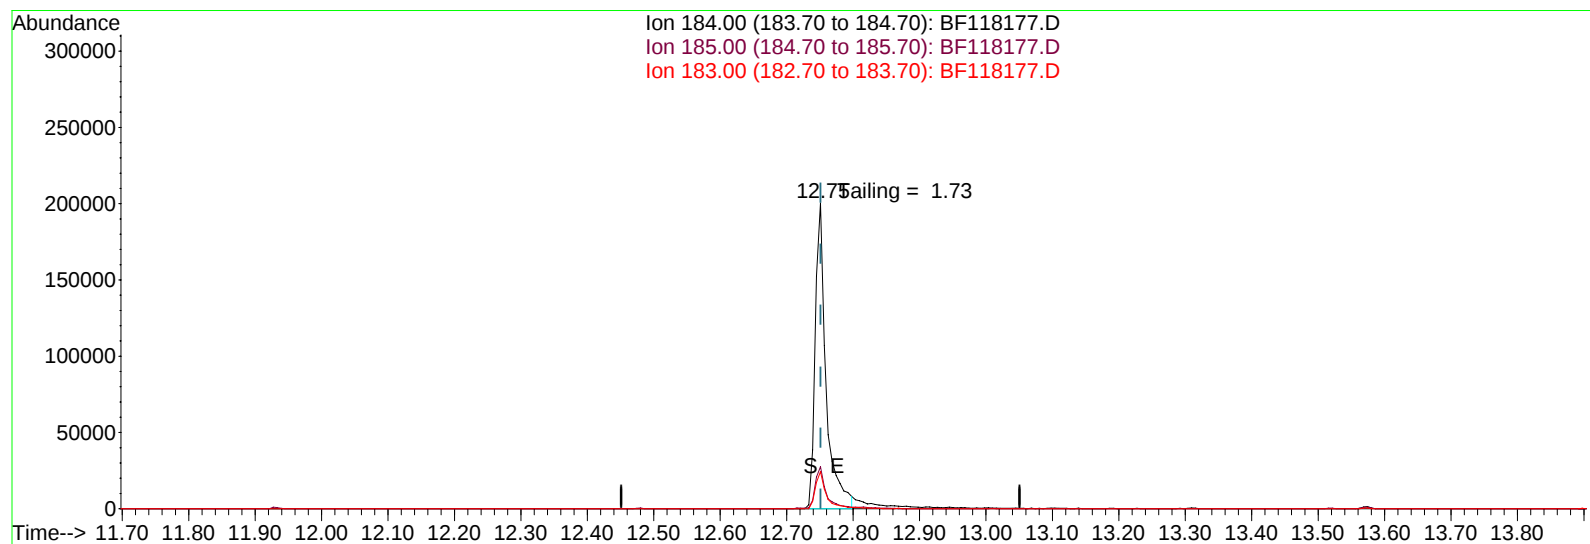

(77) Benzidine

12.751min (-0.000) 8013.38ng

response 244917

Ion	Exp%	Act%
184.00	100	100
185.00	15.40	13.77
183.00	12.40	12.12
0.00	0.00	0.00