

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF121319\
 Data File : BF118193.D
 Acq On : 13 Dec 2019 18:31
 Operator : JU
 Sample : K6264-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 VNJ-239

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120619.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.922	308	312	323	rVB	46437	64462	2.60%	0.317%
2	4.451	395	402	417	rBV	1092441	1256270	50.72%	6.171%
3	5.081	502	509	512	rBV	1212201	1442992	58.26%	7.088%
4	5.481	573	577	594	rBV	633931	595942	24.06%	2.927%
5	6.492	745	749	765	rBV	1377166	1381801	55.79%	6.788%
6	6.633	769	773	784	rVB	1103415	897251	36.23%	4.407%
7	6.863	809	812	816	rBV	766747	667771	26.96%	3.280%
8	7.022	835	839	855	rVB	1819841	1502629	60.67%	7.381%
9	7.428	904	908	920	rBV	1140632	1076669	43.47%	5.289%
10	8.151	1028	1031	1046	rBV	934417	848343	34.25%	4.167%
11	9.227	1210	1214	1230	rBV	2482706	2261654	91.31%	11.109%
12	9.339	1230	1233	1241	rVB4	26697	39722	1.60%	0.195%
13	9.627	1278	1282	1292	rBV	89271	103457	4.18%	0.508%
14	9.839	1310	1318	1327	rBV7	18250	62621	2.53%	0.308%
15	9.916	1327	1331	1347	rVB	1034689	1030997	41.63%	5.064%
16	10.704	1462	1465	1473	rBV	291685	309507	12.50%	1.520%
17	11.139	1535	1539	1543	rBV	70466	74838	3.02%	0.368%
18	11.298	1562	1566	1571	rVB2	21954	32493	1.31%	0.160%
19	11.404	1581	1584	1592	rBV	1055457	1050982	42.43%	5.163%
20	11.927	1670	1673	1679	rBV	74415	89704	3.62%	0.441%
21	11.992	1680	1684	1686	rVV	35673	39036	1.58%	0.192%
22	12.445	1758	1761	1766	rBV2	55907	56206	2.27%	0.276%
23	12.645	1789	1795	1799	rBV5	16757	28319	1.14%	0.139%
24	12.998	1850	1855	1858	rBV	2614249	2476776	100.00%	12.166%
25	13.562	1947	1951	1955	rVB3	24279	26719	1.08%	0.131%
26	13.886	2002	2006	2016	rBV	331808	391772	15.82%	1.924%
27	14.057	2031	2035	2043	rVB	809066	793126	32.02%	3.896%
28	14.209	2058	2061	2068	rVB	100081	86134	3.48%	0.423%
29	14.515	2110	2113	2120	rVB	131612	130260	5.26%	0.640%
30	14.827	2162	2166	2170	rBV	139730	136573	5.51%	0.671%
31	14.904	2175	2179	2182	rBV	73631	73217	2.96%	0.360%
32	15.174	2220	2225	2228	rBV	129017	147658	5.96%	0.725%
33	15.551	2284	2289	2301	rVB	595373	891374	35.99%	4.379%
34	16.003	2362	2366	2372	rVV	74045	103959	4.20%	0.511%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF121319\
Data File : BF118193.D
Acq On : 13 Dec 2019 18:31
Operator : JU
Sample : K6264-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
VNJ-239

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120619.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	16.062	2372	2376	2385	rVB6	36705	68689	2.77%	0.337%
36	16.521	2448	2454	2458	rBV2	42011	80520	3.25%	0.396%
37	17.133	2553	2558	2565	rVB7	17427	37478	1.51%	0.184%


Sum of corrected areas: 20357921

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF121319\
Data File : BF118193.D
Acq On : 13 Dec 2019 18:31
Operator : JU
Sample : K6264-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
VNJ-239

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF120619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

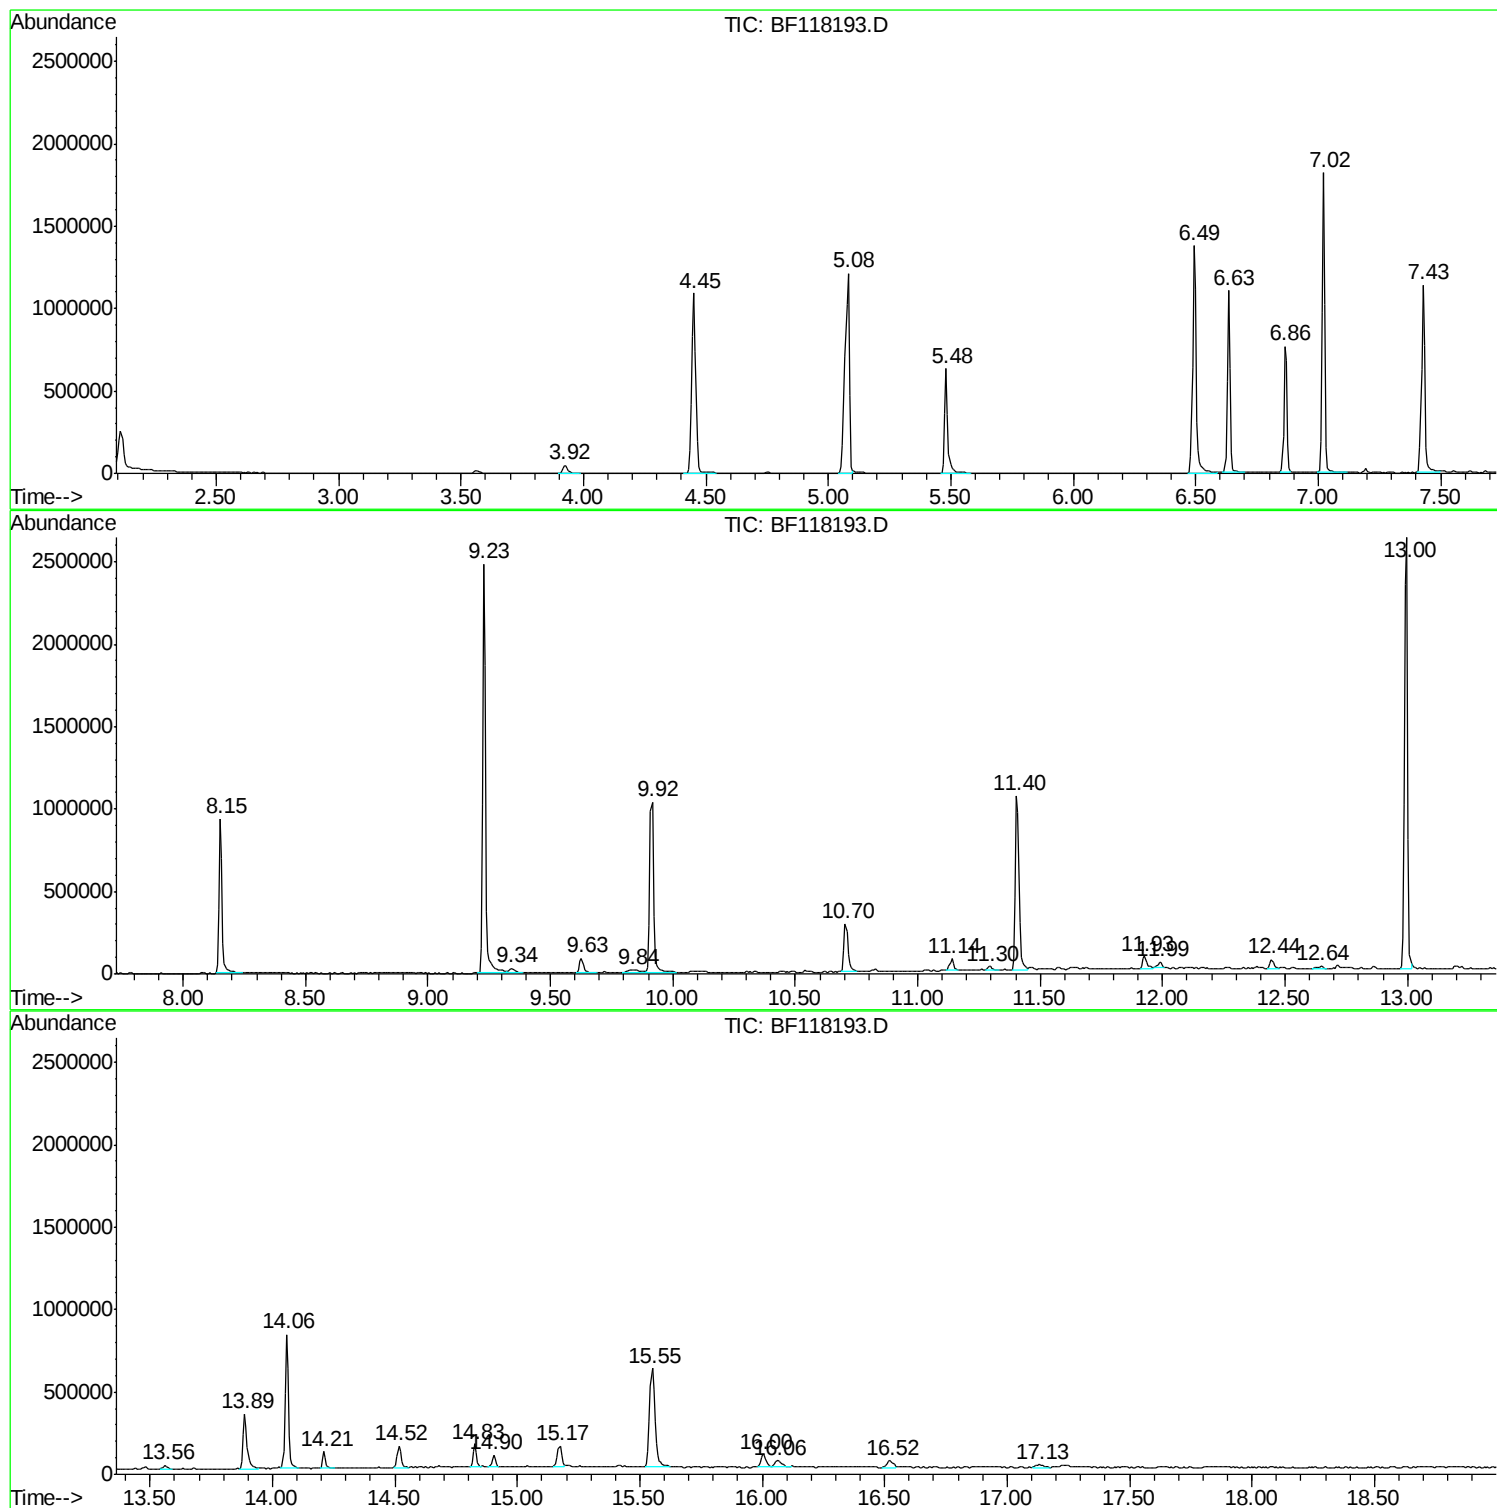

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF121319\
Data_File : BF118193.D
Acq_On : 13-Dec-2019 18:311
Operator : JUJ
Sample : K6264-011
Misc :
ALS_Vial : 17 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
VNJ-239

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120619.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
