


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF121319\
 Data File : BF118177.D
 Acq On : 13 Dec 2019 10:14
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 06 17:34:43 2019

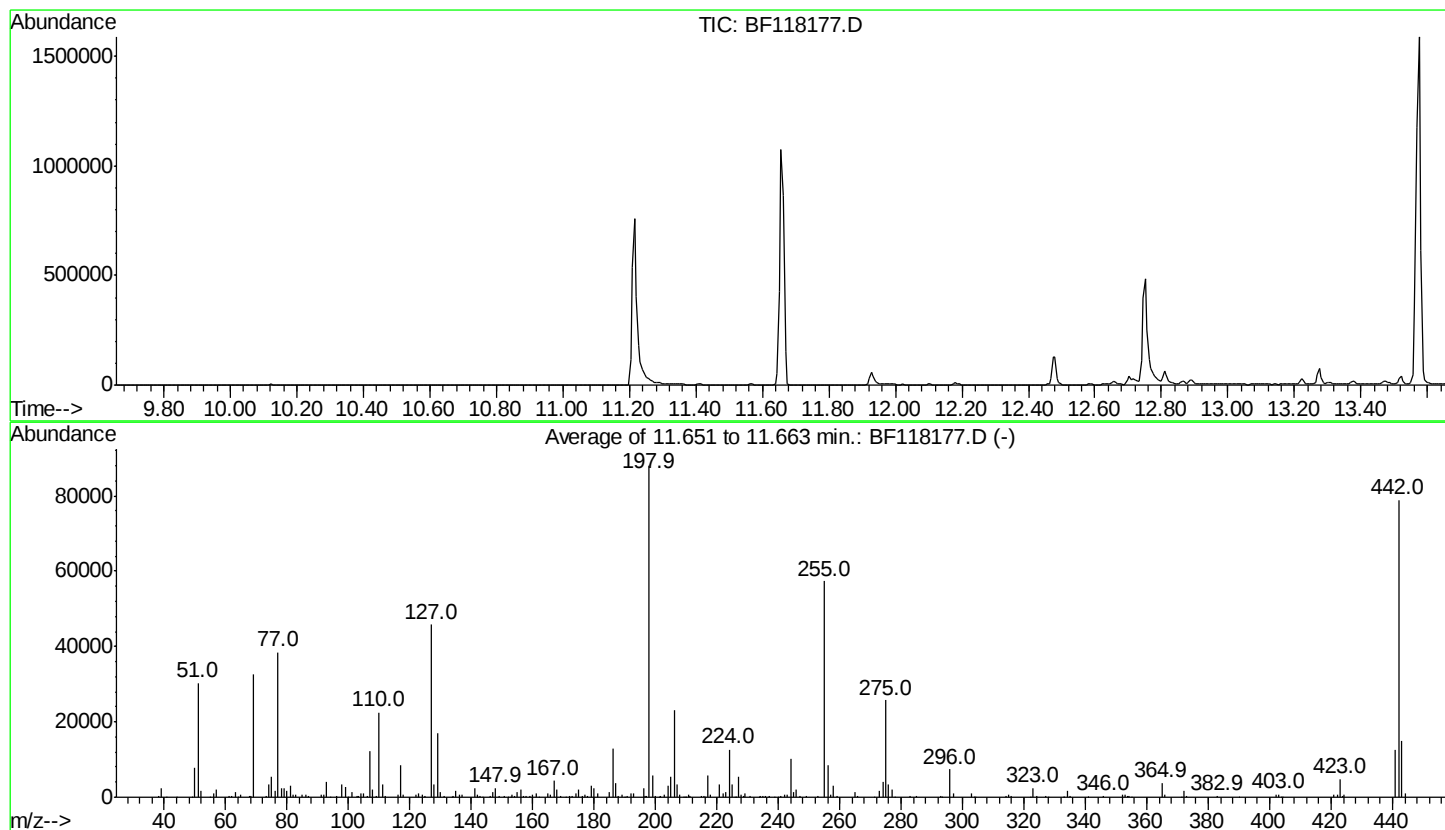

AutoFind: Scans 1626, 1627, 1628; Background Corrected with Scan 1621

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.6	30418	PASS
68	69	0.00	2	1.5	480	PASS
69	198	0.00	100	37.1	32661	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.0	45794	PASS
197	198	0.00	2	0.3	271	PASS
198	198	100	100	100.0	88010	PASS
199	198	5	9	6.6	5782	PASS
275	198	10	60	29.3	25769	PASS
365	198	1	100	4.3	3792	PASS
441	198	0.01	100	14.5	12732	PASS
442	198	50	100	89.8	78989	PASS
443	442	15	24	18.9	14907	PASS