

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121322\
 Data File : BF131626.D
 Acq On : 13 Dec 2022 22:31
 Operator : CG\JU
 Sample : N5985-01DL 10X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OR-02-120922DL

Quant Time: Dec 14 03:36:26 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 14 03:22:29 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.881	152	60724	20.000	ng	0.00
21) Naphthalene-d8	8.169	136	219464	20.000	ng	# 0.00
39) Acenaphthene-d10	9.933	164	122851	20.000	ng	0.00
64) Phenanthrene-d10	11.427	188	216766	20.000	ng	0.00
76) Chrysene-d12	14.086	240	138917	20.000	ng	# 0.00
86) Perylene-d12	15.592	264	145655	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.487	112	43869	12.052	ng	-0.01
7) Phenol-d6	6.504	99	58701	12.307	ng	-0.02
23) Nitrobenzene-d5	7.445	82	39770	6.851	ng	-0.01
42) 2,4,6-Tribromophenol	10.727	330	11589	8.491	ng	0.00
45) 2-Fluorobiphenyl	9.245	172	64447	6.614	ng	-0.01
79) Terphenyl-d14	13.021	244	56031	5.531	ng	0.00
Target Compounds						Qvalue
25) Isophorone	7.445	82	39769	4.253	ng	# 69
31) Naphthalene	8.192	128	310289	25.102	ng	99
33) 4-Chloroaniline	8.192	127	40117	8.658	ng	# 29
35) Caprolactam	8.886	113	2034	2.078	ng	# 1
37) 2-Methylnaphthalene	8.886	142	75359	8.915	ng	100
38) 1-Methylnaphthalene	8.986	142	42090	5.187	ng	95
51) 2,6-Dinitrotoluene	9.933	165	17124	8.857	ng	# 11
52) Acenaphthene	9.969	154	72577	9.324	ng	98
55) Dibenzofuran	10.139	168	105978	9.635	ng	95
56) 4-Nitrophenol	10.139	139	42379	32.886	ng	# 1
58) Fluorene	10.486	166	131017	14.653	ng	97
71) Phenanthrene	11.457	178	741081	61.336	ng	99
72) Anthracene	11.504	178	239676	20.389	ng	98
73) Carbazole	11.663	167	57924	6.037	ng	97
75) Fluoranthene	12.651	202	704501	56.625	ng	98
78) Pyrene	12.886	202	607884	44.378	ng	98
81) Benzo(a)anthracene	14.074	228	287573	28.665	ng	98
83) Chrysene	14.110	228	215158	22.559	ng	98
84) Bis(2-ethylhexyl)phtha...	14.074	149	2120	3.400	ng	# 93
85) Di-n-octyl phthalate	14.674	149	1606	5.381	ng	# 52
87) Indeno(1,2,3-cd)pyrene	17.109	276	103937	8.744	ng	96
88) Benzo(b)fluoranthene	15.151	252	372452	38.798	ng	98
89) Benzo(k)fluoranthene	15.151	252	372452	37.171	ng	# 97
90) Benzo(a)pyrene	15.527	252	223464	27.276	ng	98
91) Dibenzo(a,h)anthracene	17.298	278	21113	2.158	ng	99
92) Benzo(g,h,i)perylene	17.574	276	93359	9.495	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121322\
Data File : BF131626.D
Acq On : 13 Dec 2022 22:31
Operator : CG\JU
Sample : N5985-01DL 10X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OR-02-120922DL

Quant Time: Dec 14 03:36:26 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 14 03:22:29 2022
Response via : Initial Calibration




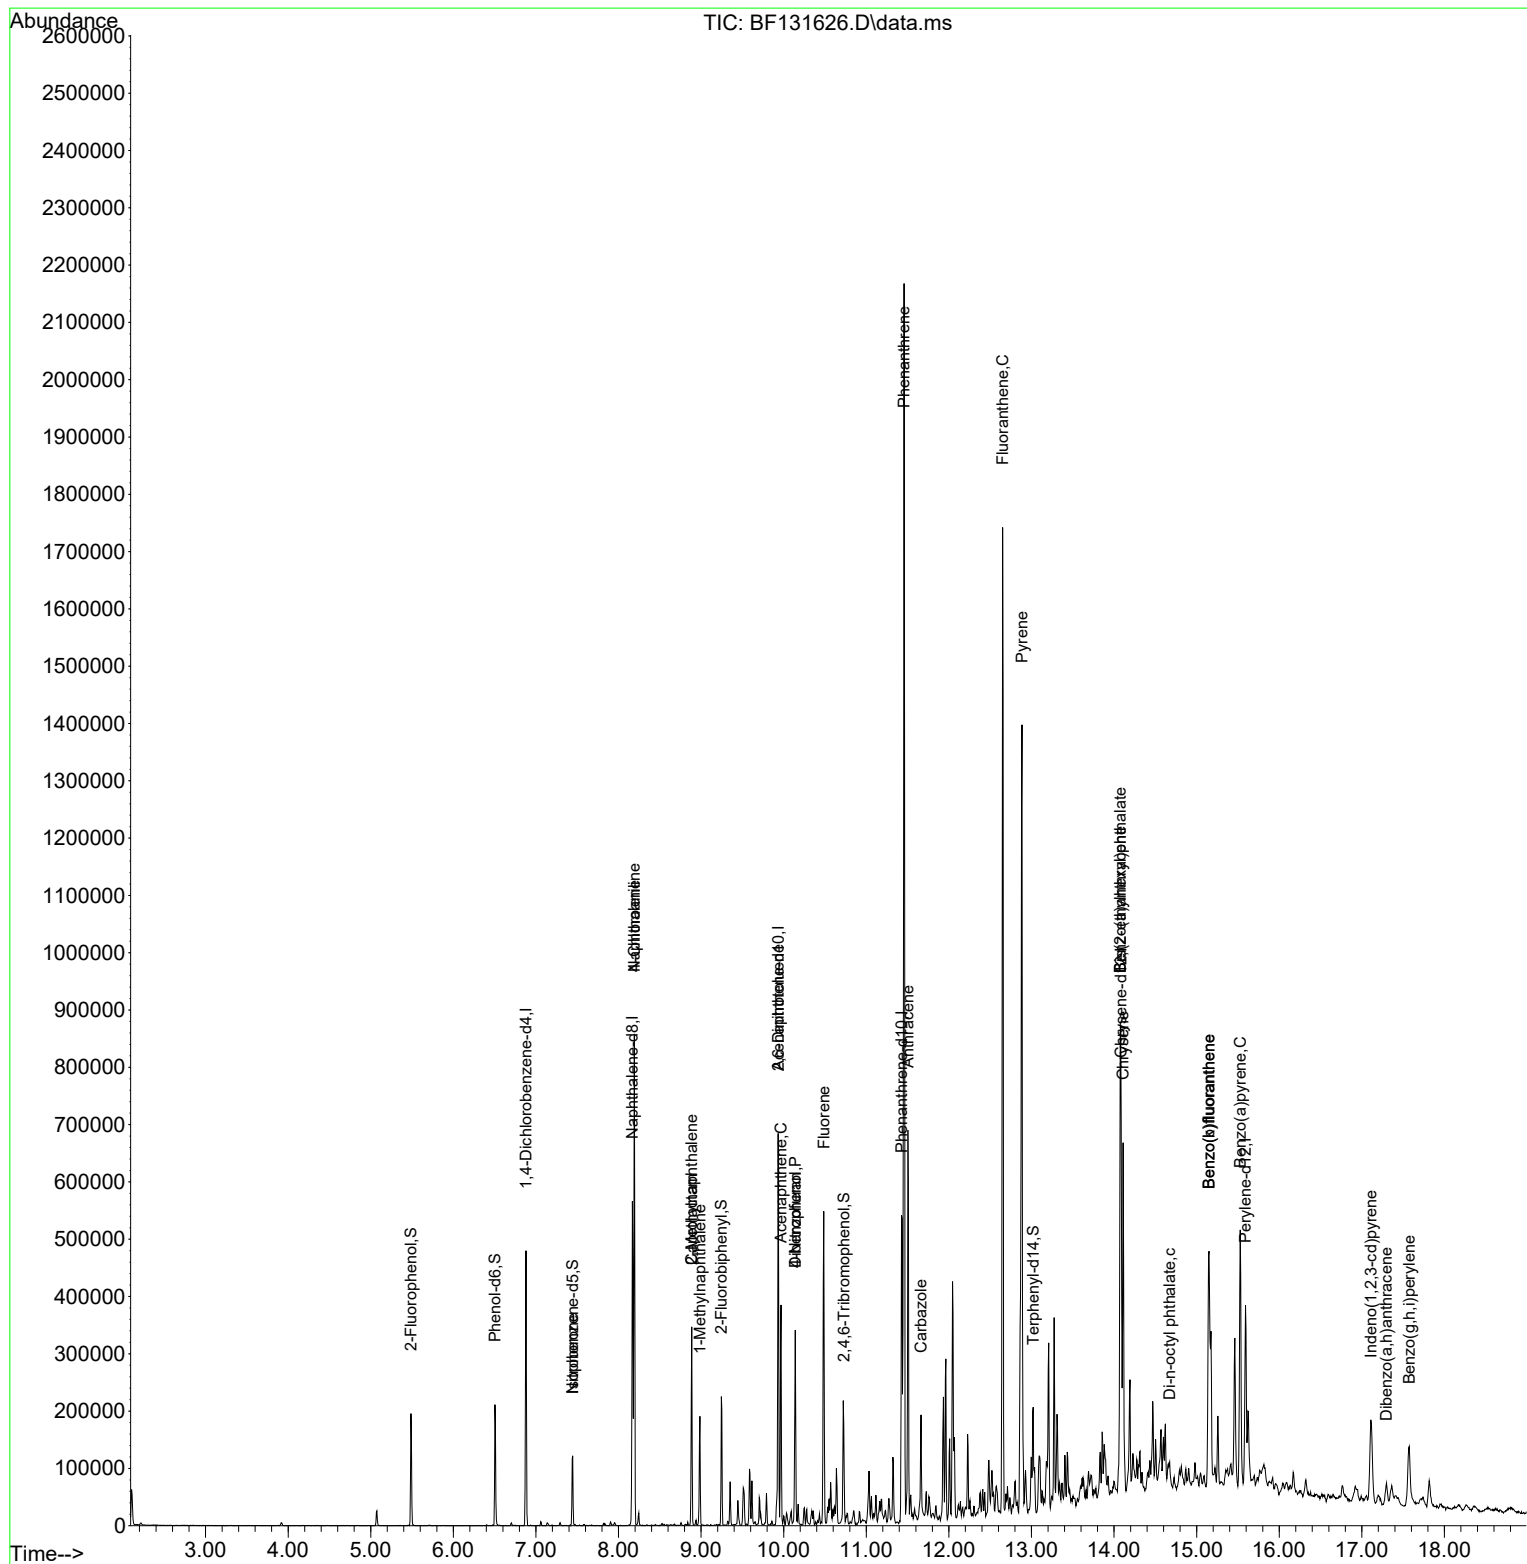




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.881 min Scan# 81
Delta R.T. -0.005 min
Lab File: BF131626.D
Acq: 13 Dec 2022 22:31




Instrument :
BNA_F
ClientSampleId :
OR-02-120922DL


Tgt Ion:152 Resp: 60724
Ion Ratio Lower Upper
152 100
150 149.9 116.7 175.1
115 68.2 54.6 82.0

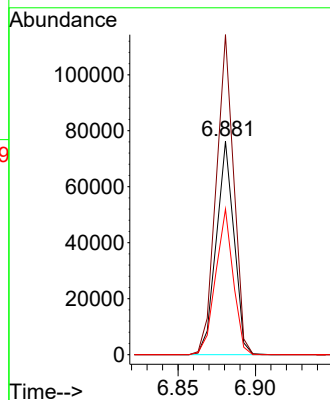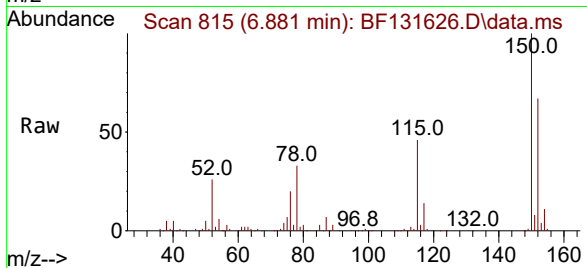

#5
2-Fluorophenol
Concen: 12.052 ng
RT: 5.487 min Scan# 578
Delta R.T. -0.012 min
Lab File: BF131626.D
Acq: 13 Dec 2022 22:31

Tgt Ion:112 Resp: 43869
Ion Ratio Lower Upper
112 100
64 70.2 54.5 81.7
63 37.6 31.9 47.9


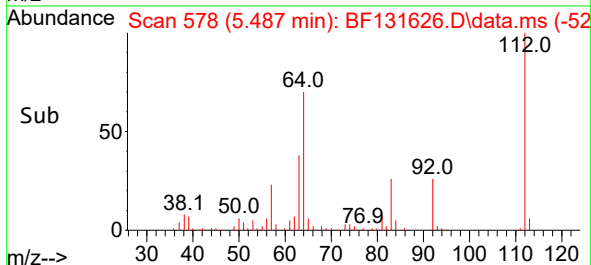
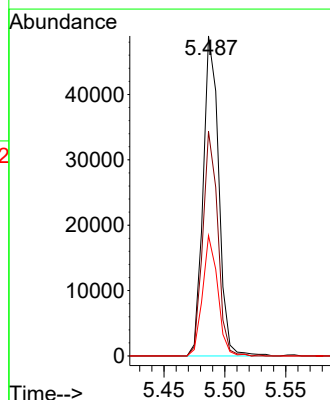
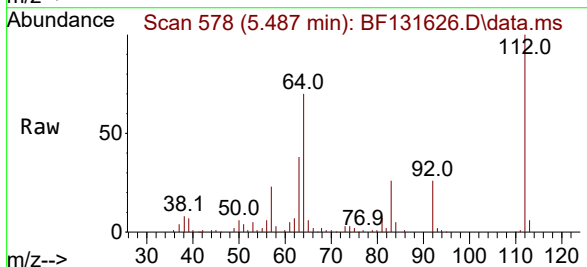




#7
Phenol-d6
Concen: 12.307 ng
RT: 6.504 min Scan# 71
Delta R.T. -0.018 min
Lab File: BF131626.D
Acq: 13 Dec 2022 22:31




Instrument :
BNA_F
ClientSampleId :
OR-02-120922DL


Tgt Ion: 99 Resp: 58701
Ion Ratio Lower Upper
99 100
42 20.8 17.9 26.9
71 45.1 37.2 55.8

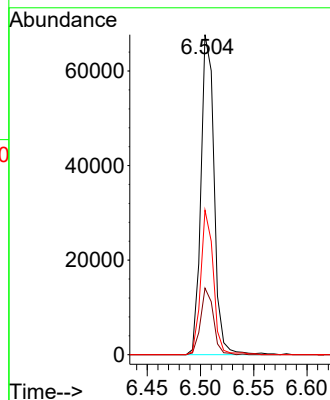

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.169 min Scan# 1034
Delta R.T. -0.006 min
Lab File: BF131626.D
Acq: 13 Dec 2022 22:31

Tgt Ion: 136 Resp: 219464
Ion Ratio Lower Upper
136 100
137 10.9 8.1 12.1
54 8.9 6.0 9.0
68 6.6 3.8 5.8

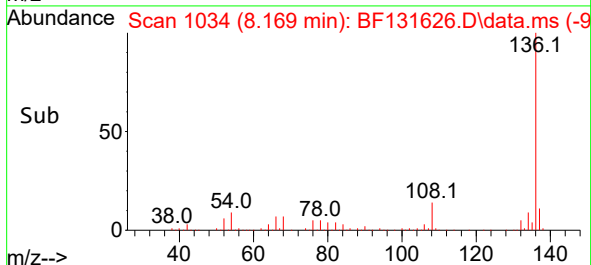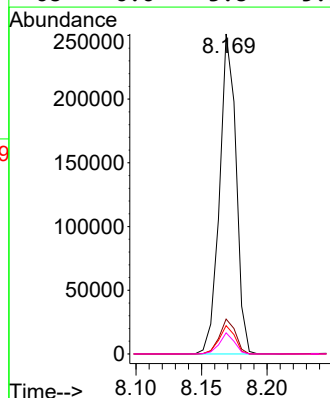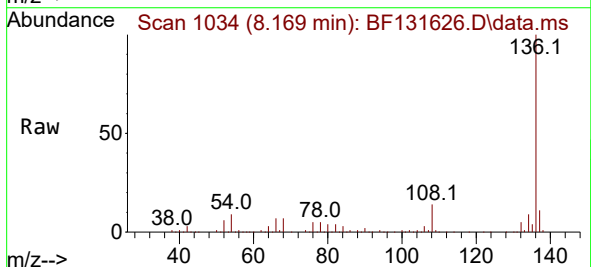



#23

Nitrobenzene-d5

Concen: 6.851 ng

RT: 7.445 min Scan# 911

Delta R.T. -0.012 min

Lab File: BF131626.D

Acq: 13 Dec 2022 22:31

Instrument :

BNA_F

ClientSampleId :

OR-02-120922DL





Tgt Ion: 82 Resp: 39770

Ion Ratio Lower Upper

82 100

128 35.2 26.1 39.1

54 42.3 40.6 60.8

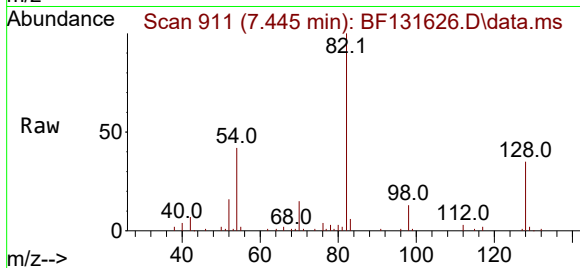

#25

Isophorone

Concen: 4.253 ng

RT: 7.445 min Scan# 911

Delta R.T. -0.265 min

Lab File: BF131626.D

Acq: 13 Dec 2022 22:31




Tgt Ion: 82 Resp: 39769


Ion Ratio Lower Upper

82 100

95 0.0 6.9 10.3#

138 0.0 11.4 17.0#


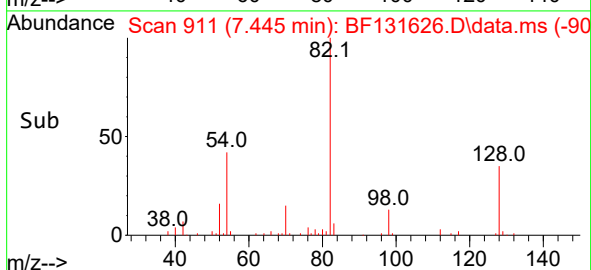
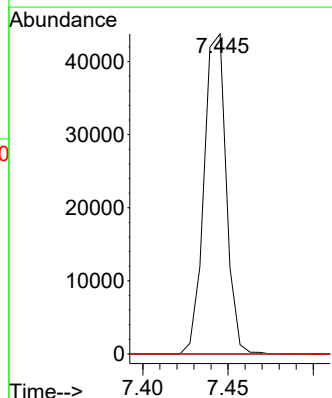
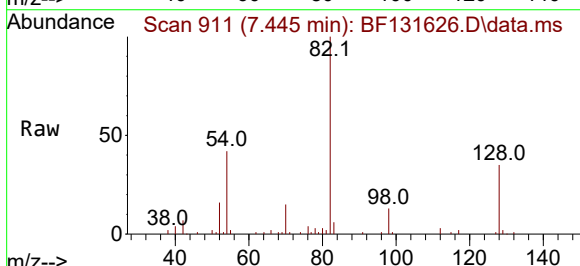




#31
Naphthalene
Concen: 25.102 ng
RT: 8.192 min Scan# 1038
Delta R.T. -0.006 min
Lab File: BF131626.D
Acq: 13 Dec 2022 22:31




Instrument :
BNA_F
ClientSampleId :
OR-02-120922DL


Tgt Ion:128 Resp: 310289
Ion Ratio Lower Upper
128 100
129 11.3 8.9 13.3
127 12.9 10.6 15.8



#33
4-Chloroaniline
Concen: 8.658 ng
RT: 8.192 min Scan# 1038
Delta R.T. -0.059 min
Lab File: BF131626.D
Acq: 13 Dec 2022 22:31

Tgt Ion:127 Resp: 40117
Ion Ratio Lower Upper
127 100
129 87.2 26.4 39.6#
65 0.0 31.9 47.9#
92 0.0 19.1 28.7#


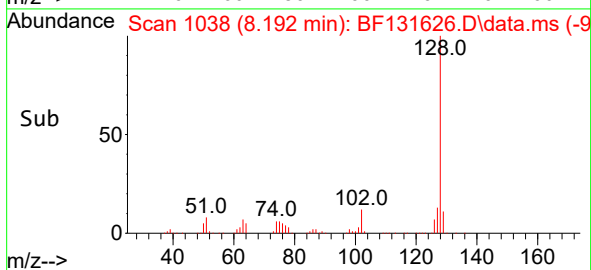

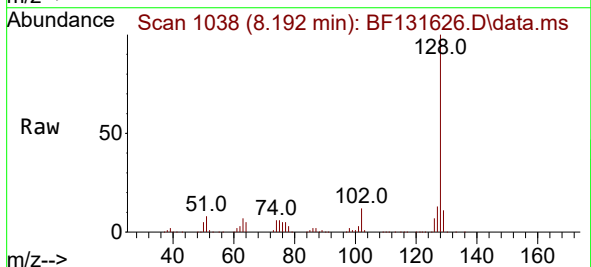




#35
 Caprolactam
 Concen: 2.078 ng
 RT: 8.886 min Scan# 1156
 Delta R.T. 0.259 min
 Lab File: BF131626.D
 Acq: 13 Dec 2022 22:31




Instrument :
 BNA_F
 ClientSampleId :
 OR-02-120922DL


Tgt Ion:113 Resp: 2034
 Ion Ratio Lower Upper
 113 100
 55 9.2 155.8 195.8#
 56 7.6 131.7 171.7#

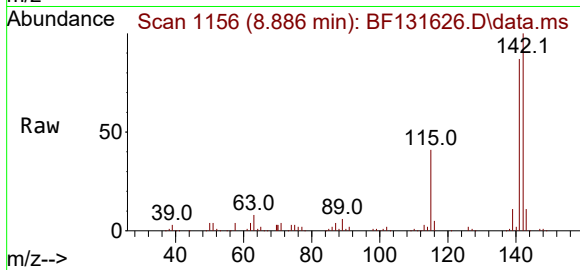

#37
 2-Methylnaphthalene
 Concen: 8.915 ng
 RT: 8.886 min Scan# 1156
 Delta R.T. -0.006 min
 Lab File: BF131626.D
 Acq: 13 Dec 2022 22:31

Tgt Ion:142 Resp: 75359
 Ion Ratio Lower Upper
 142 100
 141 87.3 69.7 104.5

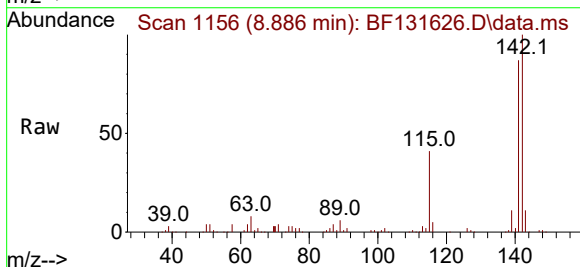



#38

1-Methylnaphthalene

Concen: 5.187 ng

RT: 8.986 min Scan# 1178

Delta R.T. -0.006 min

Lab File: BF131626.D

Acq: 13 Dec 2022 22:31

Instrument :

BNA_F

ClientSampleId :





OR-02-120922DL

Tgt Ion:142 Resp: 42090

Ion Ratio Lower Upper

142 100

141 94.8 71.9 107.9

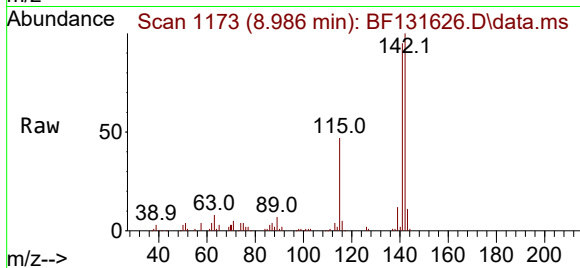

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.933 min Scan# 1334

Delta R.T. -0.006 min

Lab File: BF131626.D

Acq: 13 Dec 2022 22:31




Tgt Ion:164 Resp: 122851


Ion Ratio Lower Upper

164 100

162 100.9 81.0 121.6

160 45.2 35.0 52.6

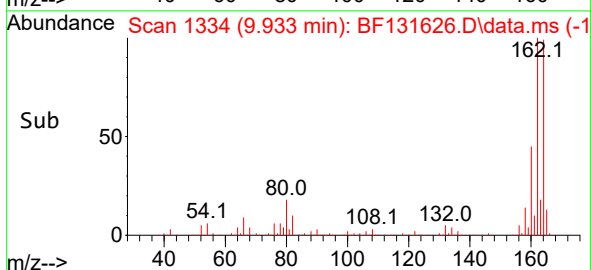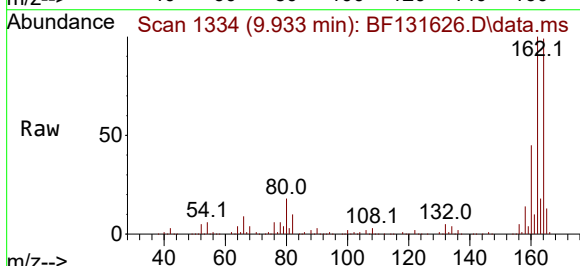



#42

2,4,6-Tribromophenol

Concen: 8.491 ng

RT: 10.727 min Scan# 1469

Delta R.T. -0.006 min

Lab File: BF131626.D


Acq: 13 Dec 2022 22:31

Instrument :

BNA_F

ClientSampleId :

OR-02-120922DL






Tgt Ion:330 Resp: 11589

Ion Ratio Lower Upper

330 100

332 93.1 78.3 117.5

141 44.3 32.6 49.0

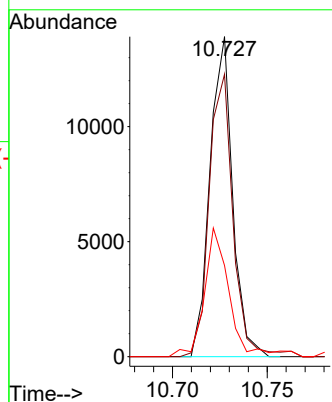

#45

2-Fluorobiphenyl

Concen: 6.614 ng

RT: 9.245 min Scan# 1217

Delta R.T. -0.012 min

Lab File: BF131626.D

Acq: 13 Dec 2022 22:31




Tgt Ion:172 Resp: 64447


Ion Ratio Lower Upper

172 100

171 32.3 28.3 42.5

170 23.1 19.3 28.9


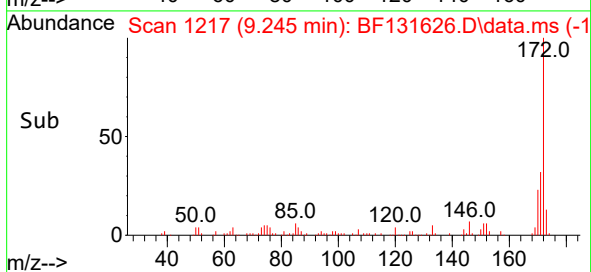






#51
2,6-Dinitrotoluene
Concen: 8.857 ng
RT: 9.933 min Scan# 11
Delta R.T. 0.206 min
Lab File: BF131626.D
Acq: 13 Dec 2022 22:31




Instrument :
BNA_F
ClientSampleId :
OR-02-120922DL


Tgt Ion:165 Resp: 17124
Ion Ratio Lower Upper
165 100
63 2.0 67.9 101.9#
89 2.0 63.2 94.8#



#52
Acenaphthene
Concen: 9.324 ng
RT: 9.969 min Scan# 1340
Delta R.T. -0.006 min
Lab File: BF131626.D
Acq: 13 Dec 2022 22:31

Tgt Ion:154 Resp: 72577
Ion Ratio Lower Upper
154 100
153 113.2 87.9 131.9
152 52.2 42.4 63.6


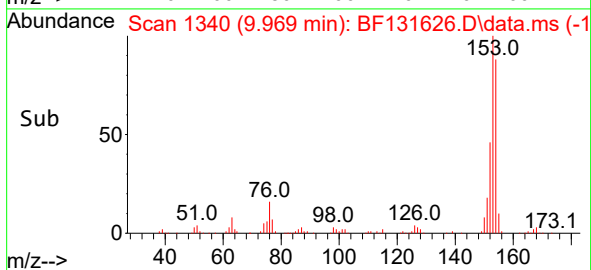

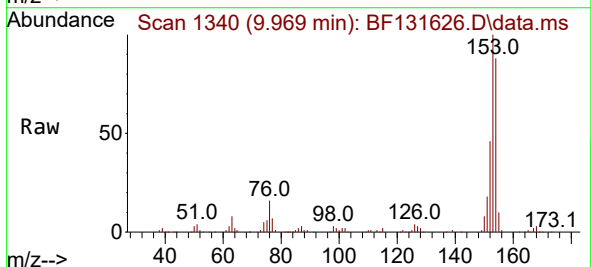




#55
Dibenzenofuran
Concen: 9.635 ng
RT: 10.139 min Scan# 1369
Delta R.T. -0.006 min
Lab File: BF131626.D
Acq: 13 Dec 2022 22:31




Instrument :
BNA_F
ClientSampleId :
OR-02-120922DL


Tgt Ion:168 Resp: 105978
Ion Ratio Lower Upper
168 100
139 38.2 33.9 50.9
169 13.6 10.7 16.1



#56
4-Nitrophenol
Concen: 32.886 ng
RT: 10.139 min Scan# 1369
Delta R.T. 0.077 min
Lab File: BF131626.D
Acq: 13 Dec 2022 22:31

Tgt Ion:139 Resp: 42379
Ion Ratio Lower Upper
139 100
109 1.2 110.2 150.2#
65 1.9 133.3 173.3#


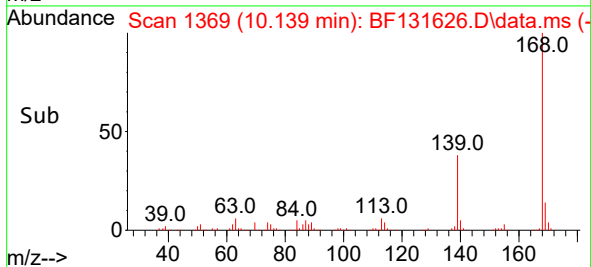

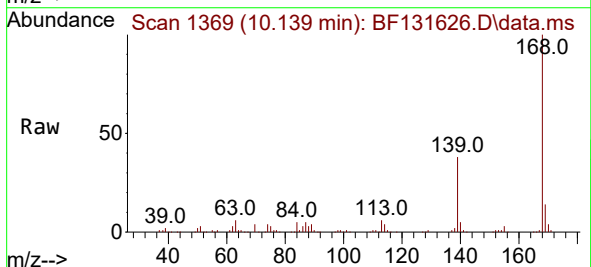


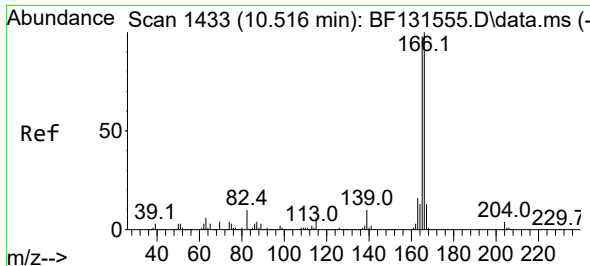

#58
Fluorene
Concen: 14.653 ng
RT: 10.486 min Scan# 14
Delta R.T. -0.006 min
Lab File: BF131626.D
Acq: 13 Dec 2022 22:31




Instrument :
BNA_F
ClientSampleId :
OR-02-120922DL


Tgt Ion:166 Resp: 131017
Ion Ratio Lower Upper
166 100
165 101.3 78.4 117.6
167 13.1 10.7 16.1

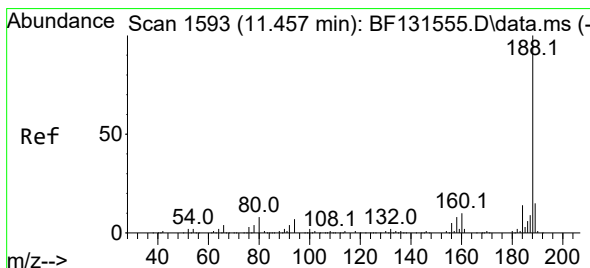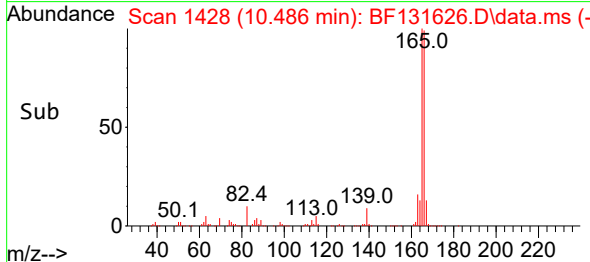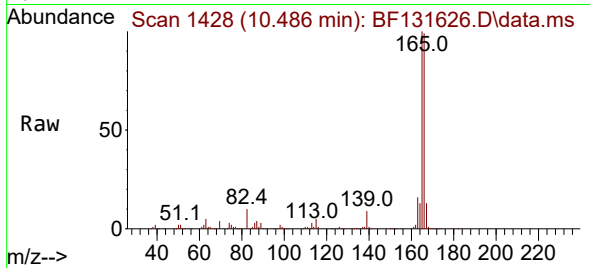

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.427 min Scan# 1588
Delta R.T. -0.006 min
Lab File: BF131626.D
Acq: 13 Dec 2022 22:31

Tgt Ion:188 Resp: 216766
Ion Ratio Lower Upper
188 100
94 7.6 5.5 8.3
80 9.8 6.6 10.0


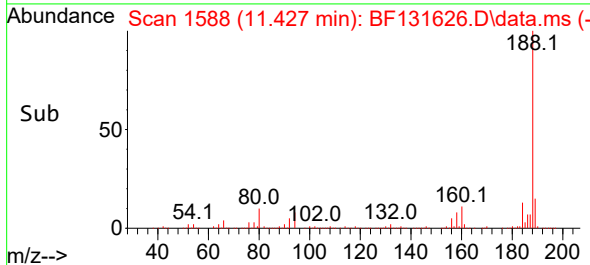

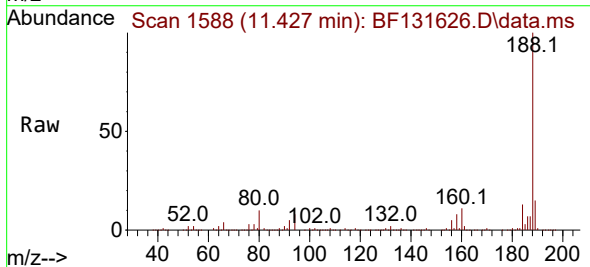




#71
Phenanthrene
Concen: 61.336 ng
RT: 11.457 min Scan# 1597
Delta R.T. -0.006 min
Lab File: BF131626.D
Acq: 13 Dec 2022 22:31




Instrument :
BNA_F
ClientSampleId :
OR-02-120922DL


Tgt Ion:178 Resp: 741081
Ion Ratio Lower Upper
178 100
176 19.8 15.4 23.0
179 15.6 12.2 18.4

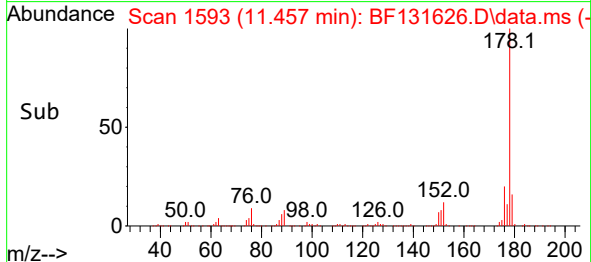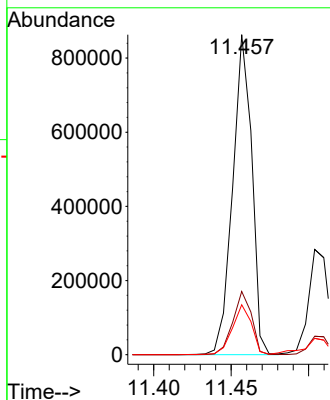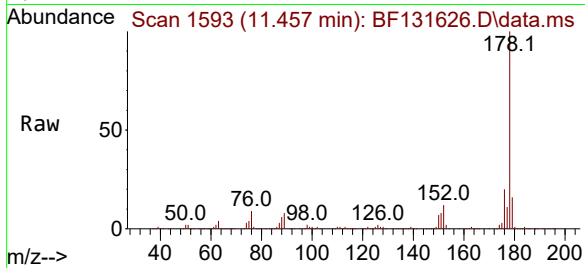

#72
Anthracene
Concen: 20.389 ng
RT: 11.504 min Scan# 1601
Delta R.T. -0.006 min
Lab File: BF131626.D
Acq: 13 Dec 2022 22:31

Tgt Ion:178 Resp: 239676
Ion Ratio Lower Upper
178 100
176 17.4 15.0 22.6
179 15.6 12.3 18.5


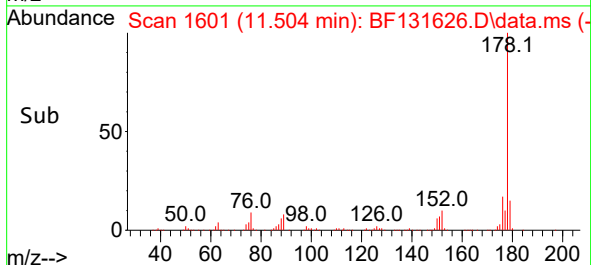
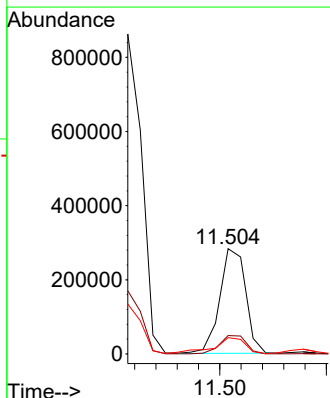
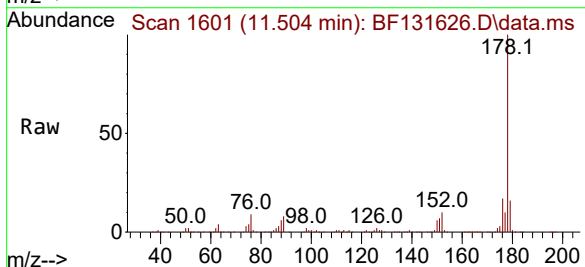




#73
Carbazole
Concen: 6.037 ng
RT: 11.663 min Scan# 1796
Delta R.T. -0.006 min
Lab File: BF131626.D
Acq: 13 Dec 2022 22:31




Instrument :
BNA_F
ClientSampleId :
OR-02-120922DL


Tgt Ion:167 Resp: 57924
Ion Ratio Lower Upper
167 100
166 20.6 17.4 26.0
139 11.9 11.0 16.4

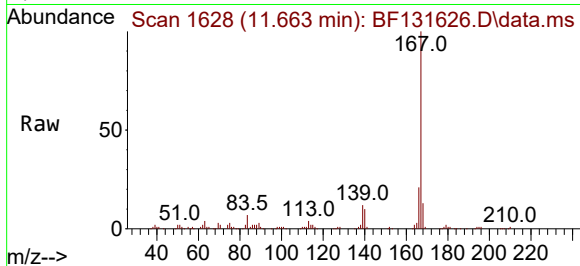

#75
Fluoranthene
Concen: 56.625 ng
RT: 12.651 min Scan# 1796
Delta R.T. 0.000 min
Lab File: BF131626.D
Acq: 13 Dec 2022 22:31

Tgt Ion:202 Resp: 704501
Ion Ratio Lower Upper
202 100
101 9.2 0.0 27.7
203 17.5 0.0 37.7

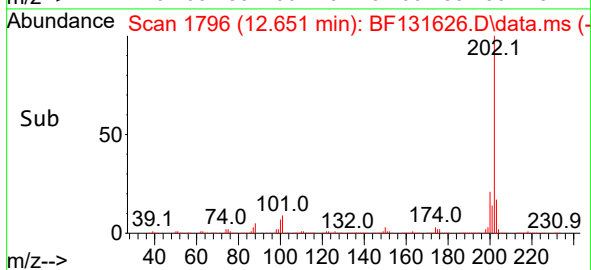



#76

Chrysene-d12

Concen: 20.000 ng

RT: 14.086 min Scan# 2040

Delta R.T. 0.000 min

Lab File: BF131626.D

Acq: 13 Dec 2022 22:31

Instrument :

BNA_F

ClientSampleId :

OR-02-120922DL





Tgt Ion:240 Resp: 138917

Ion Ratio Lower Upper

240 100

120 7.3 4.6 7.0#

236 26.4 20.2 30.2

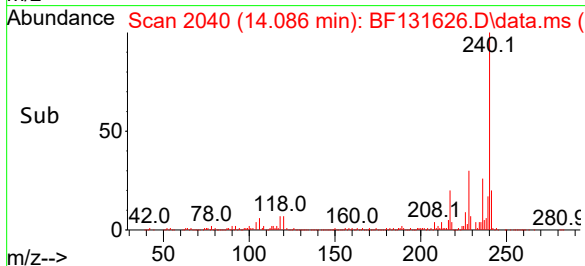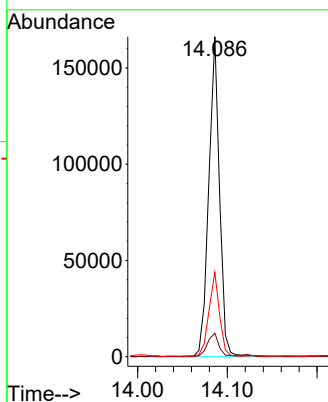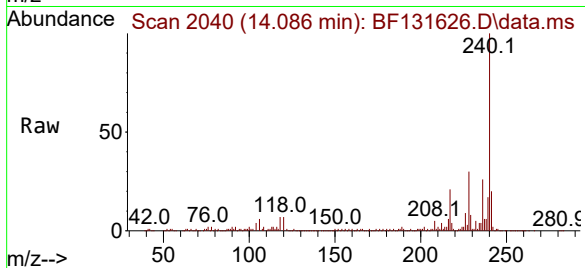

#78

Pyrene

Concen: 44.378 ng

RT: 12.886 min Scan# 1836

Delta R.T. 0.000 min

Lab File: BF131626.D

Acq: 13 Dec 2022 22:31




Tgt Ion:202 Resp: 607884


Ion Ratio Lower Upper

202 100

200 20.5 16.7 25.1

203 18.2 13.8 20.6

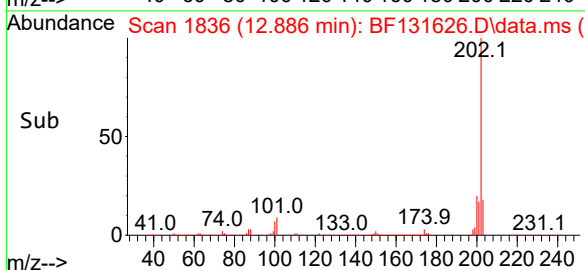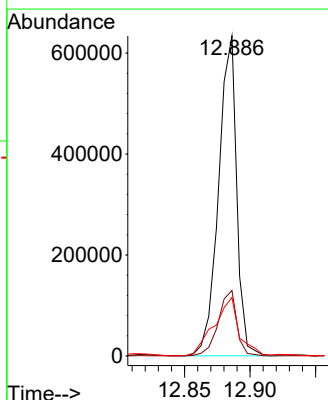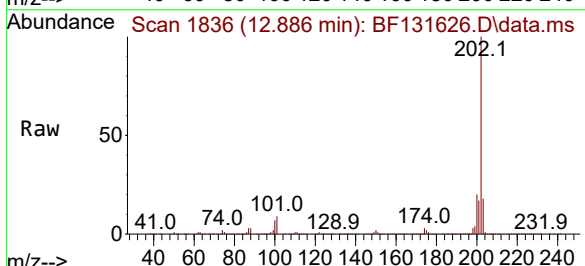



#79

Terphenyl-d14

Concen: 5.531 ng

RT: 13.021 min Scan# 1859

Delta R.T. -0.006 min

Lab File: BF131626.D


Acq: 13 Dec 2022 22:31

Instrument :

BNA_F

ClientSampleId :

OR-02-120922DL






Tgt Ion:244 Resp: 56031

Ion Ratio Lower Upper

244 100

212 7.2 6.5 9.7

122 7.0 7.1 10.7#

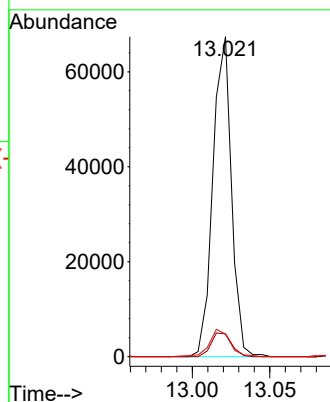

#81

Benzo(a)anthracene

Concen: 28.665 ng

RT: 14.074 min Scan# 2038

Delta R.T. -0.006 min

Lab File: BF131626.D

Acq: 13 Dec 2022 22:31




Tgt Ion:228 Resp: 287573


Ion Ratio Lower Upper

228 100

226 27.6 21.5 32.3

229 21.1 15.8 23.6

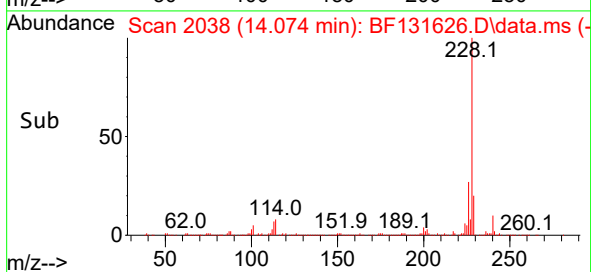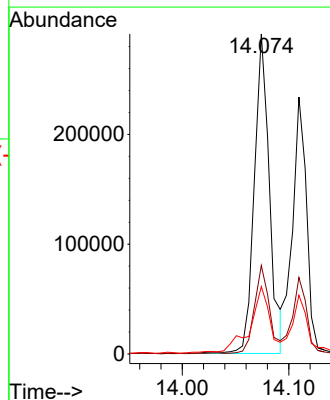

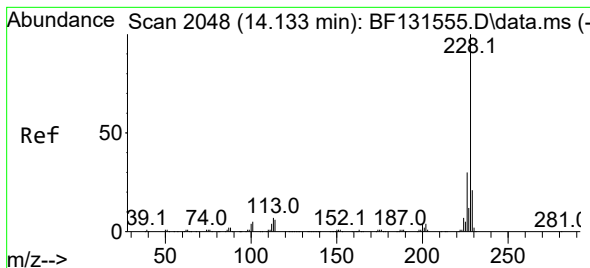

#83

Chrysene

Concen: 22.559 ng

RT: 14.110 min Scan# 2044

Delta R.T. -0.006 min

Lab File: BF131626.D

Acq: 13 Dec 2022 22:31

Instrument :

BNA_F

ClientSampleId :

OR-02-120922DL





Tgt Ion:228 Resp: 215158

Ion Ratio Lower Upper

228 100

226 29.8 23.9 35.9

229 22.8 16.7 25.1

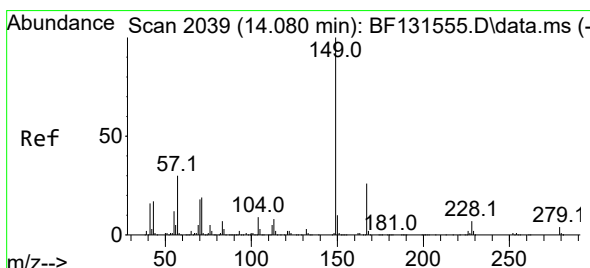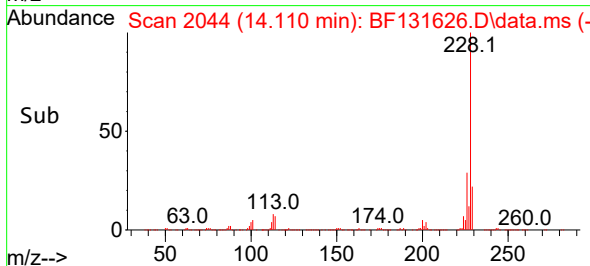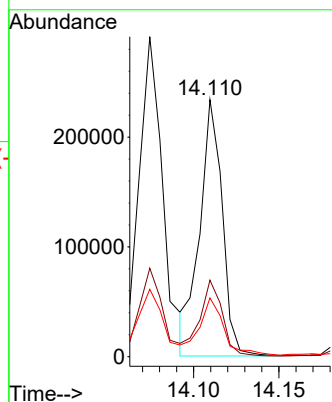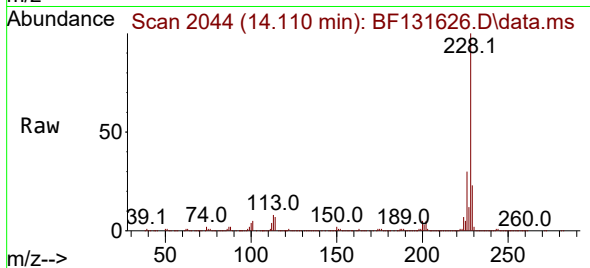

#84

Bis(2-ethylhexyl)phthalate

Concen: 3.400 ng

RT: 14.074 min Scan# 2038

Delta R.T. 0.012 min

Lab File: BF131626.D

Acq: 13 Dec 2022 22:31




Tgt Ion:149 Resp: 2120


Ion Ratio Lower Upper

149 100

167 23.0 20.8 31.2

279 0.0 3.3 4.9#


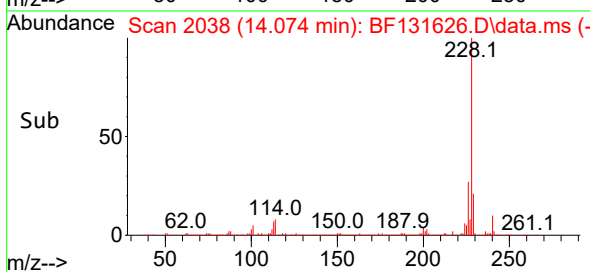
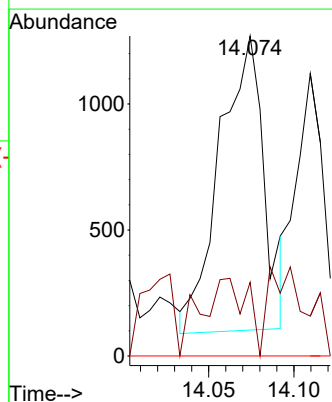
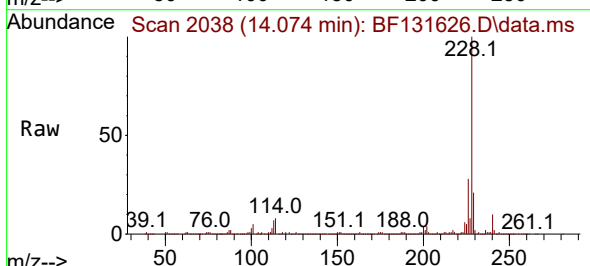




#85
Di-n-octyl phthalate
Concen: 5.381 ng
RT: 14.674 min Scan# 2145
Delta R.T. -0.006 min
Lab File: BF131626.D
Acq: 13 Dec 2022 22:31




Instrument :
BNA_F
ClientSampleId :
OR-02-120922DL


Tgt Ion:149 Resp: 1606
Ion Ratio Lower Upper
149 100
167 24.5 1.2 1.8#
43 28.4 8.6 13.0#



#86
Perylene-d12
Concen: 20.000 ng
RT: 15.592 min Scan# 2296
Delta R.T. 0.000 min
Lab File: BF131626.D
Acq: 13 Dec 2022 22:31

Tgt Ion:264 Resp: 145655
Ion Ratio Lower Upper
264 100
260 22.5 20.6 30.8
265 21.7 16.8 25.2


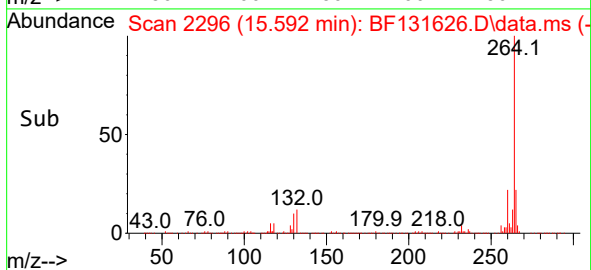

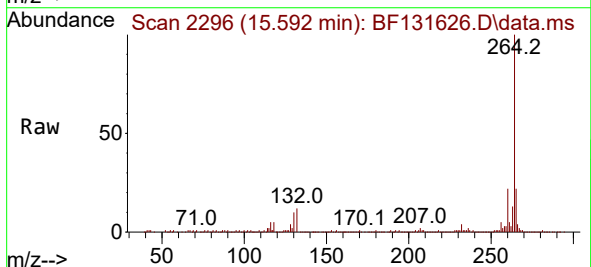




#87
Indeno(1,2,3-cd)pyrene
Concen: 8.744 ng
RT: 17.109 min Scan# 21
Delta R.T. -0.012 min
Lab File: BF131626.D
Acq: 13 Dec 2022 22:31




Instrument :
BNA_F
ClientSampleId :
OR-02-120922DL


Tgt Ion:276 Resp: 103937
Ion Ratio Lower Upper
276 100
138 14.0 12.7 19.1
277 23.3 20.0 30.0

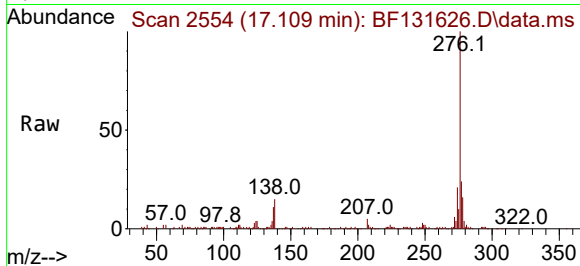

#88
Benzo(b)fluoranthene
Concen: 38.798 ng
RT: 15.151 min Scan# 2221
Delta R.T. 0.000 min
Lab File: BF131626.D
Acq: 13 Dec 2022 22:31

Tgt Ion:252 Resp: 372452
Ion Ratio Lower Upper
252 100
253 23.4 17.7 26.5
125 7.4 5.6 8.4


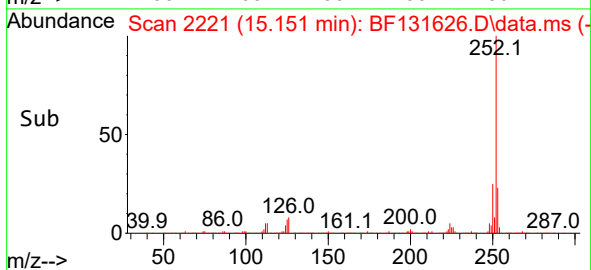

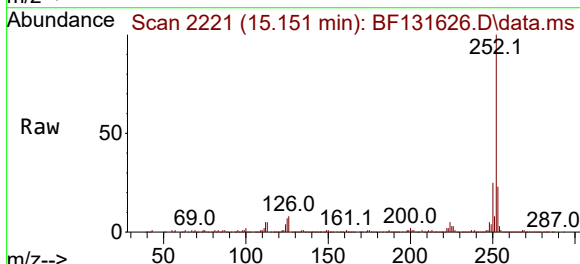




#89
Benzo(k)fluoranthene
Concen: 37.171 ng
RT: 15.151 min Scan# 211
Delta R.T. -0.029 min
Lab File: BF131626.D
Acq: 13 Dec 2022 22:31




Instrument :
BNA_F
ClientSampleId :
OR-02-120922DL


Tgt Ion:252 Resp: 372452
Ion Ratio Lower Upper
252 100
253 23.4 17.7 26.5
125 7.4 4.9 7.3#

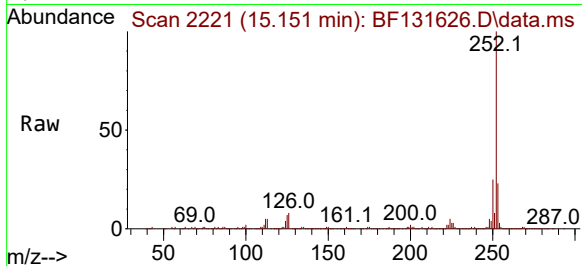

#90
Benzo(a)pyrene
Concen: 27.276 ng
RT: 15.527 min Scan# 2285
Delta R.T. 0.000 min
Lab File: BF131626.D
Acq: 13 Dec 2022 22:31

Tgt Ion:252 Resp: 223464
Ion Ratio Lower Upper
252 100
253 22.6 17.5 26.3
125 8.0 5.6 8.4


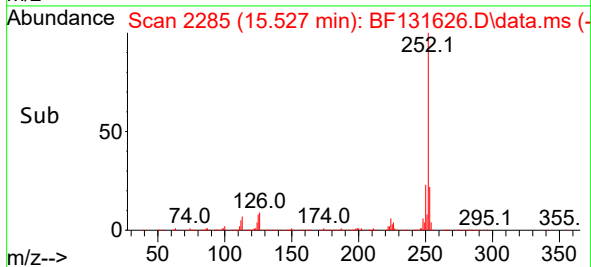

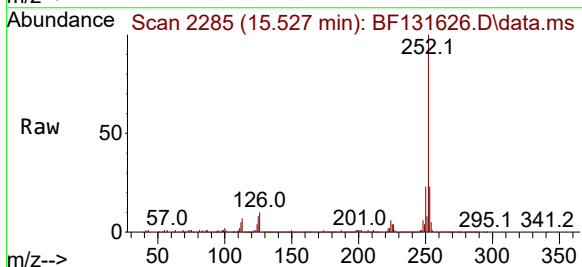




#91
Dibenzo(a,h)anthracene
Concen: 2.158 ng
RT: 17.298 min Scan# 21113
Delta R.T. 0.159 min
Lab File: BF131626.D
Acq: 13 Dec 2022 22:31

Instrument :
BNA_F
ClientSampleId :
OR-02-120922DL

Tgt Ion:278 Resp: 21113
Ion Ratio Lower Upper
278 100
139 11.4 8.9 13.3
279 24.5 19.0 28.6

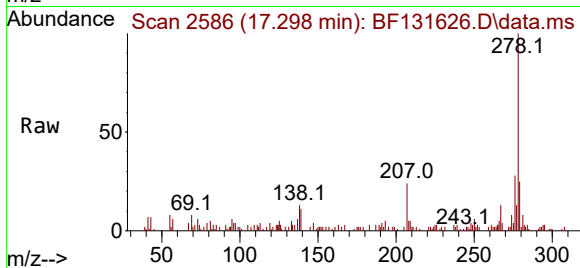

#92
Benzo(g,h,i)perylene
Concen: 9.495 ng
RT: 17.574 min Scan# 2633
Delta R.T. -0.018 min
Lab File: BF131626.D
Acq: 13 Dec 2022 22:31

Tgt Ion:276 Resp: 93359
Ion Ratio Lower Upper
276 100
277 24.7 19.0 28.6
138 14.9 10.7 16.1

