


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121322\
 Data File : BF131609.D
 Acq On : 13 Dec 2022 11:57
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 14 03:22:29 2022

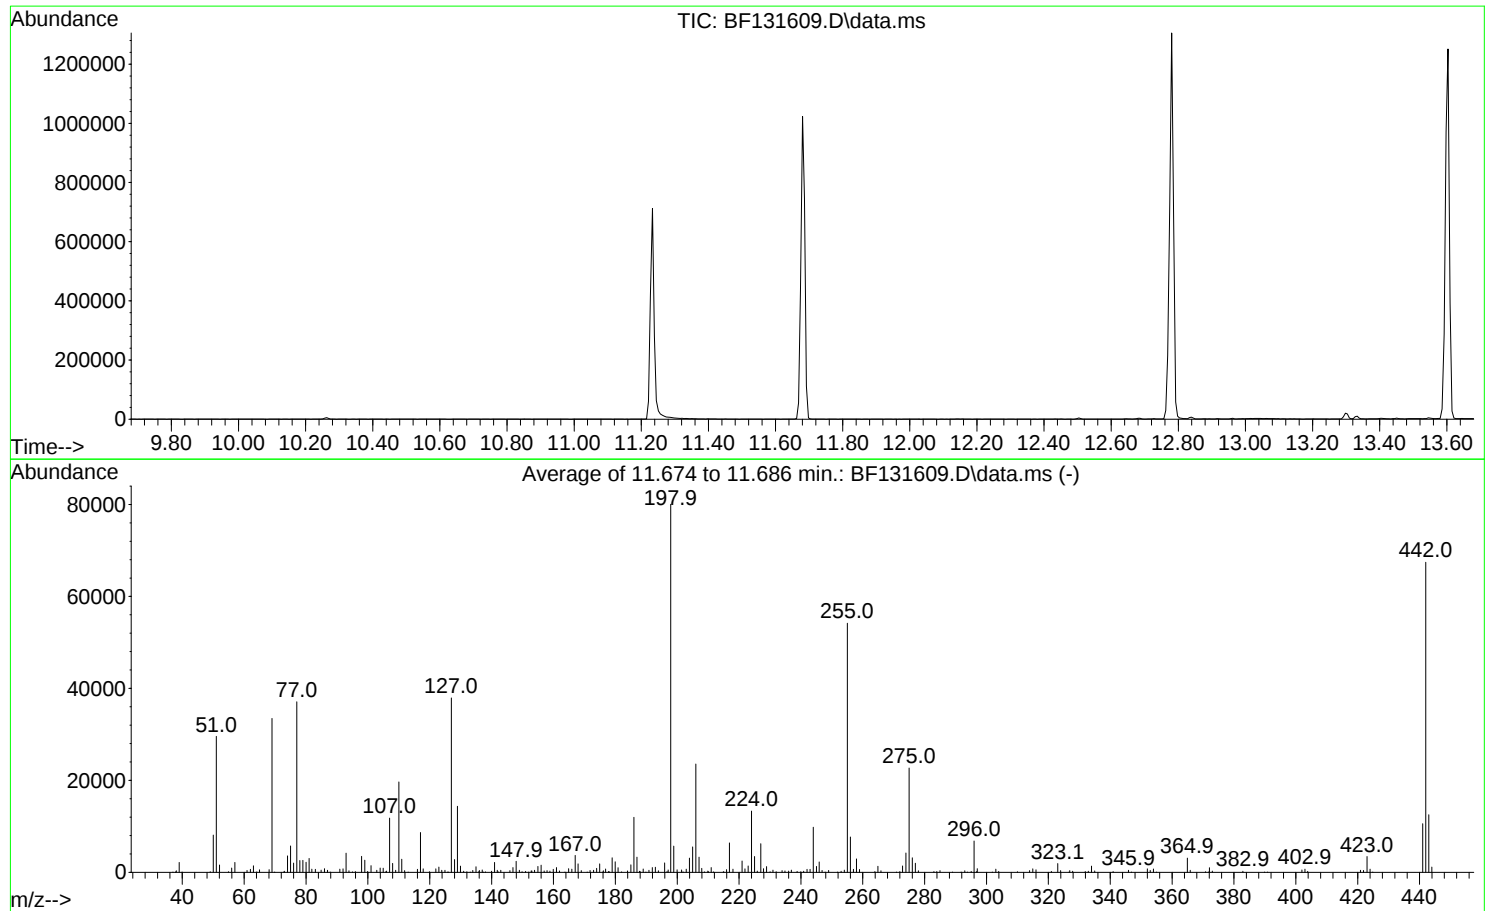

AutoFind: Scans 1630, 1631, 1632; Background Corrected with Scan 1625

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.0	29571	PASS
68	69	0.00	2	1.7	577	PASS
69	198	0.00	100	41.8	33469	PASS
70	69	0.00	2	0.2	65	PASS
127	198	10	80	47.4	37917	PASS
197	198	0.00	2	0.6	511	PASS
198	198	100	100	100.0	80013	PASS
199	198	5	9	7.1	5699	PASS
275	198	10	60	28.4	22688	PASS
365	198	1	100	3.8	3078	PASS
441	198	0.01	100	13.2	10561	PASS
442	442	50	100	100.0	67440	PASS
443	442	15	24	18.6	12523	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
12/13/2022	BNA_F	<u>BF131609.D</u>
Compound Name	Response	Retention Time
DDT	206704	13.604
DDD	5773	13.298
DDE	498	12.963
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6271	212975	2.94

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121322\
Data File : BF131609.D
Acq On : 13 Dec 2022 11:57
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 14 06:44:38 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 14 03:22:29 2022
Response via : Initial Calibration

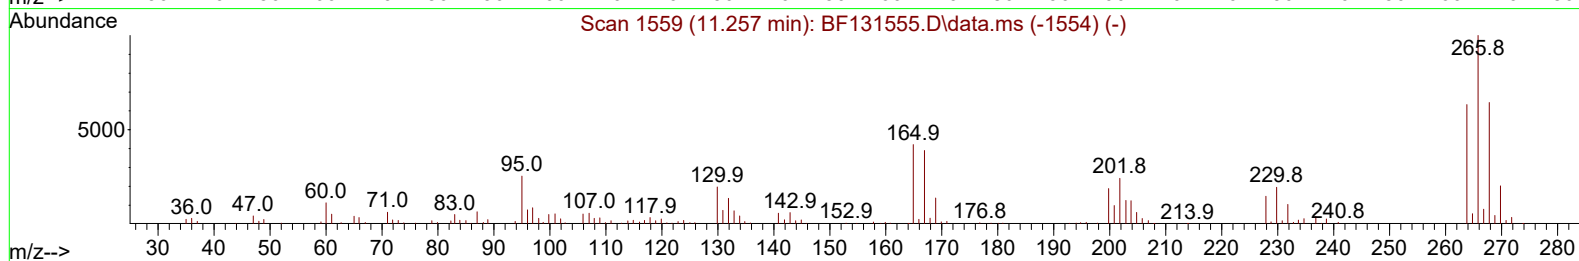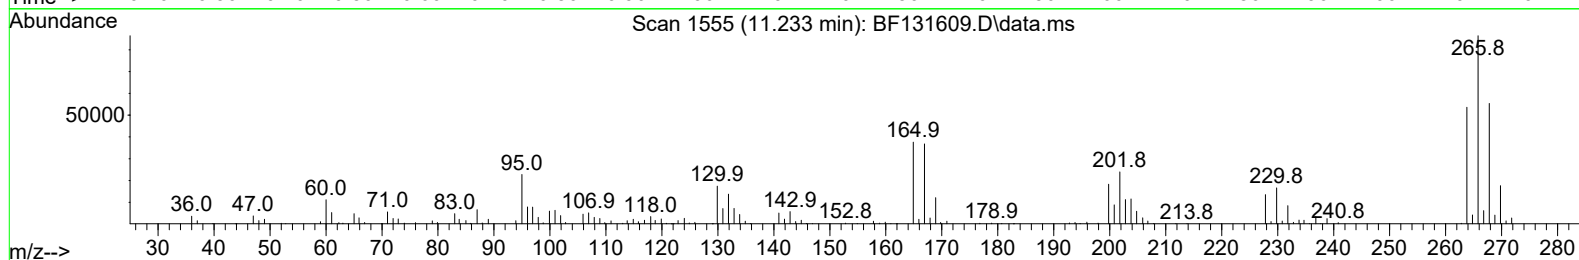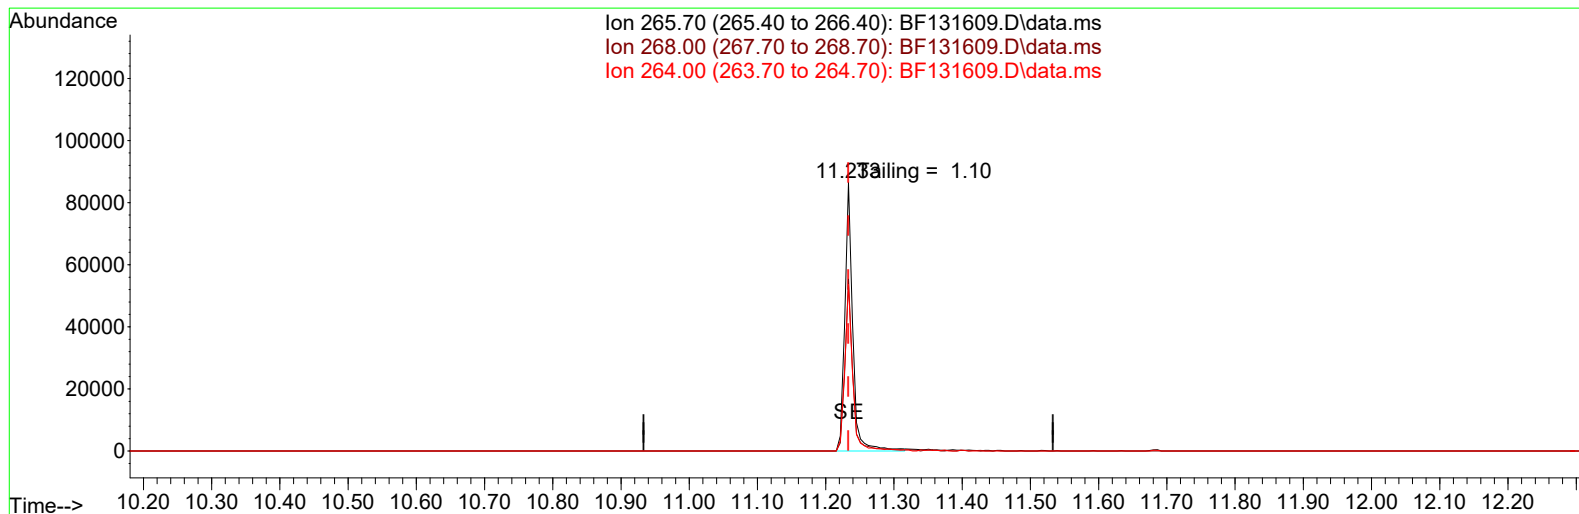

TIC: BF131609.D\data.ms

(70) Pentachlorophenol (C)

11.233min (+ 0.000) 23531.23 ng




response 69449

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.40	64.03
264.00	63.40	62.06
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121322\
Data File : BF131609.D
Acq On : 13 Dec 2022 11:57
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 14 06:44:38 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 14 03:22:29 2022
Response via : Initial Calibration

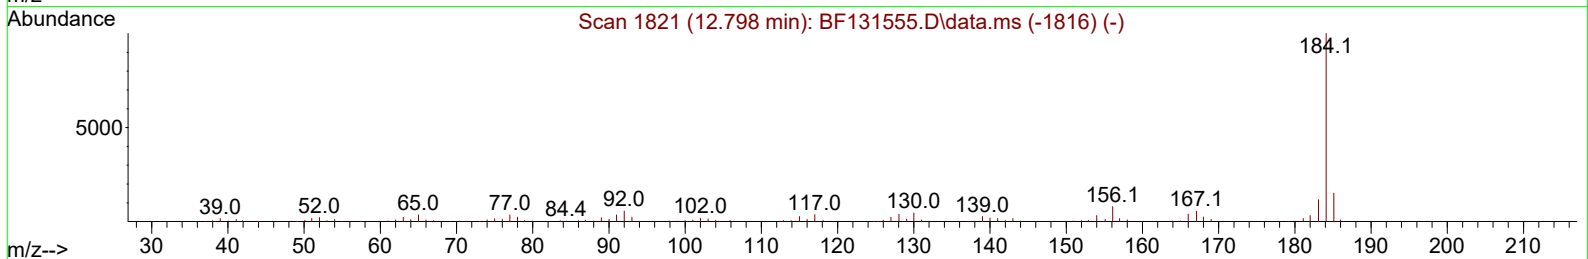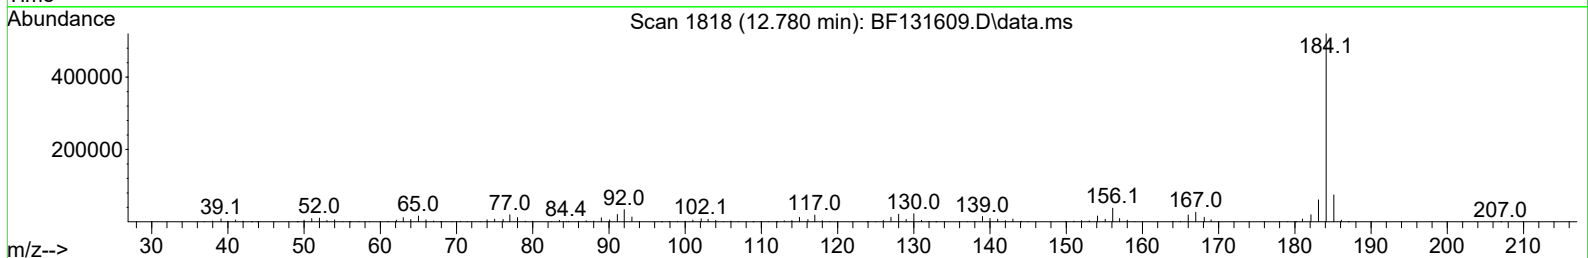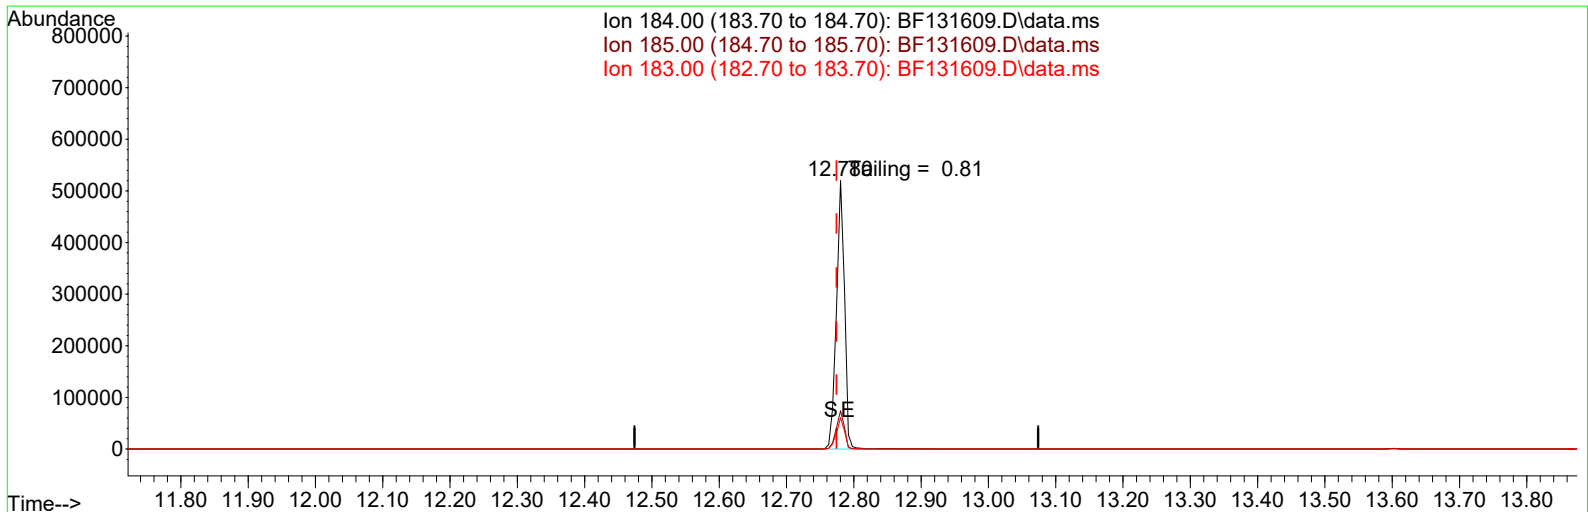

TIC: BF131609.D\data.ms

(77) Benzidine

12.780min (+ 0.006) 0.00 ng

response 435275

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.29
183.00	11.60	11.71
0.00	0.00	0.00