

Data Path : Z:\HPCHEM1\BNA F\DATA\BF121415\
 Data File : BF083786.D
 Acq On : 14 Dec 2015 23:19
 Operator : UM/IZ
 Sample : G4779-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 W-35

Quant Time: Dec 15 03:05:09 2015
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121315.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 14 01:30:12 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.90	152	110287	20.00	ng	-0.02
21) Naphthalene-d8	8.18	136	404379	20.00	ng	-0.03
38) Acenaphthene-d10	9.94	164	216029	20.00	ng	-0.02
63) Phenanthrene-d10	11.41	188	368430	20.00	ng	-0.03
75) Chrysene-d12	14.04	240	303333	20.00	ng	-0.03
86) Perylene-d12	15.48	264	227440	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.49	112	332072	48.57	ng	-0.03
7) Phenol-d6	6.52	99	304548	35.18	ng	-0.02
23) Nitrobenzene-d5	7.46	82	585278	80.97	ng	-0.02
41) 2,4,6-Tribromophenol	10.73	330	314308	142.78	ng	-0.02
44) 2-Fluorobiphenyl	9.26	172	1196575	79.60	ng	-0.02
78) Terphenyl-d14	13.00	244	992451	70.38	ng	-0.02


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF121415\
Data File : BF083786.D
Acq On : 14 Dec 2015 23:19
Operator : UM/IZ
Sample : G4779-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
W-35

Quant Time: Dec 15 03:05:09 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 14 01:30:12 2015
Response via : Initial Calibration

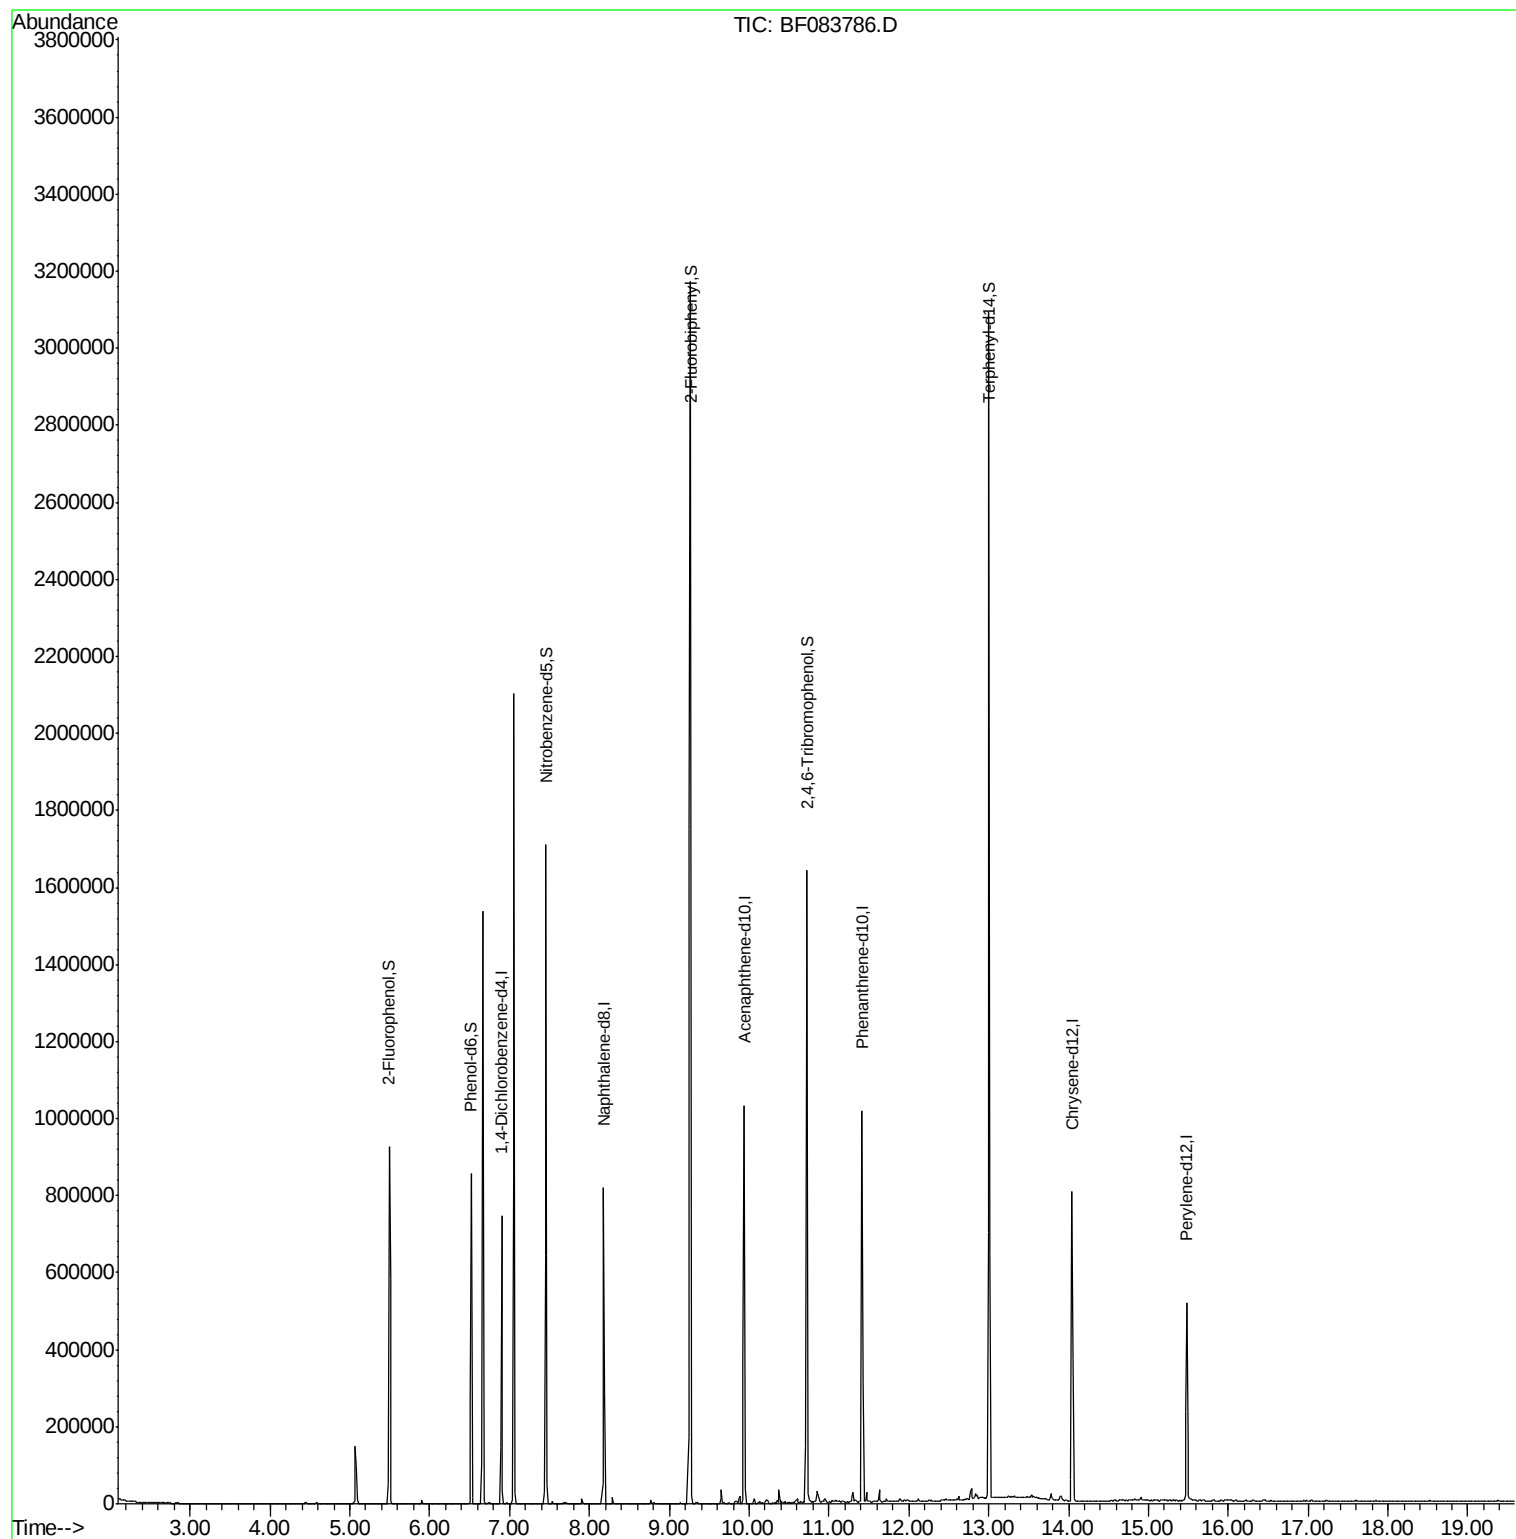

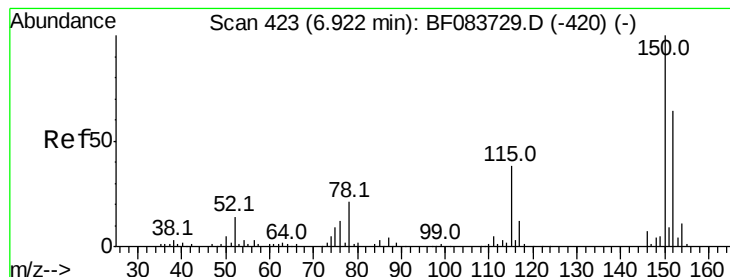

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.90 min Scan# 421

Delta R.T. -0.02 min

Lab File: BF083786.D

Acq: 14 Dec 2015 23:19

Instrument :

BNA_F

ClientSampleId :

W-35


Tot Ion:152 Resp: 110287

Ion Ratio Lower Upper

152 100

150 156.3 126.5 189.7




115 61.1 52.3 78.5

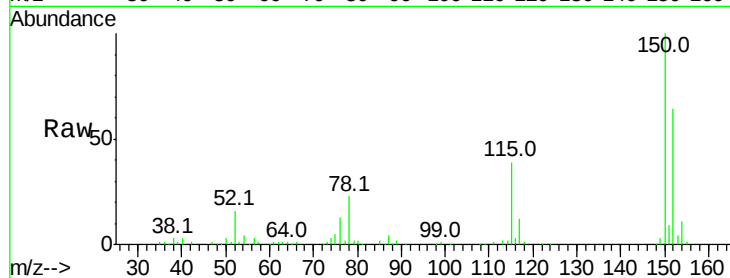

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

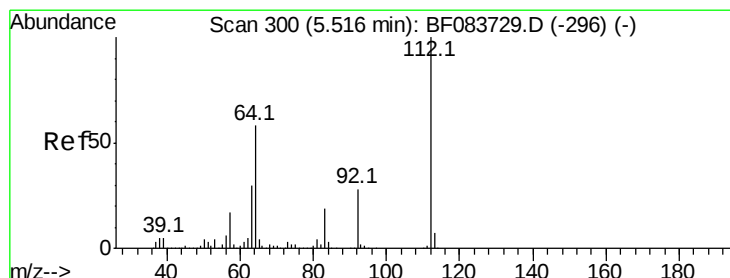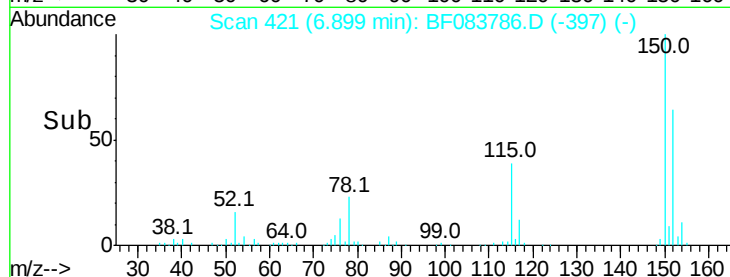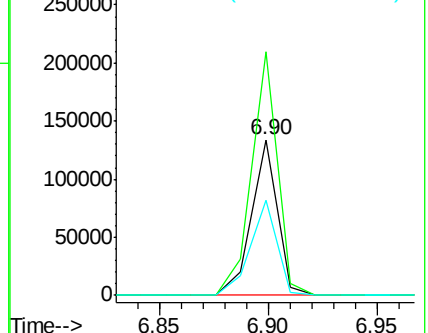

#5

2-Fluorophenol

Concen: 48.57 ng

RT: 5.49 min Scan# 298

Delta R.T. -0.03 min

Lab File: BF083786.D

Acq: 14 Dec 2015 23:19


Tgt Ion:112 Resp: 332072

Ion Ratio Lower Upper

112 100

64 62.2 50.5 75.7



63 31.0 25.8 38.6

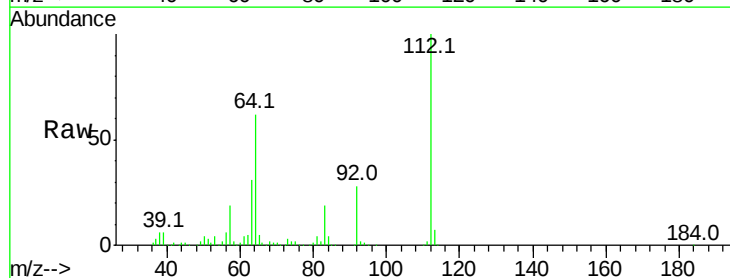


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

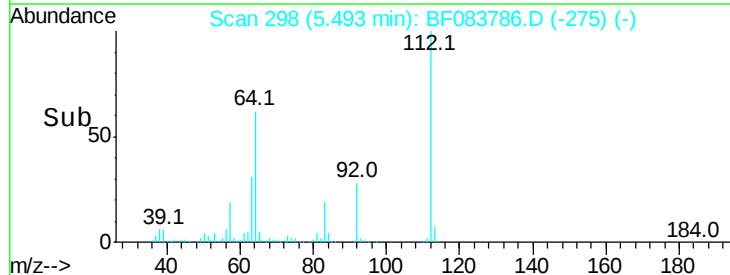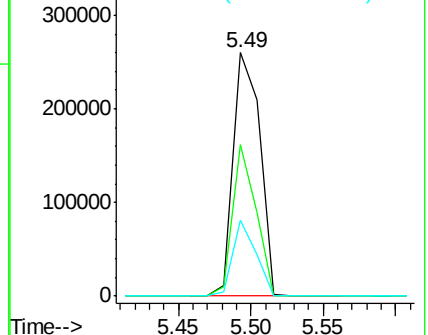

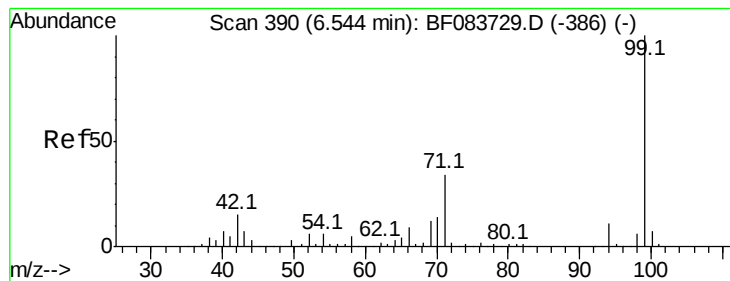

#7

Phenol-d6

Concen: 35.18 ng

RT: 6.52 min Scan# 388

Delta R.T. -0.02 min

Lab File: BF083786.D

Acq: 14 Dec 2015 23:19

Instrument :

BNA_F

ClientSampleId :

W-35


Tot Ion: 99 Resp: 304548

Ion Ratio Lower Upper

99 100

42 12.8 17.3 25.9#




71 31.8 26.6 40.0

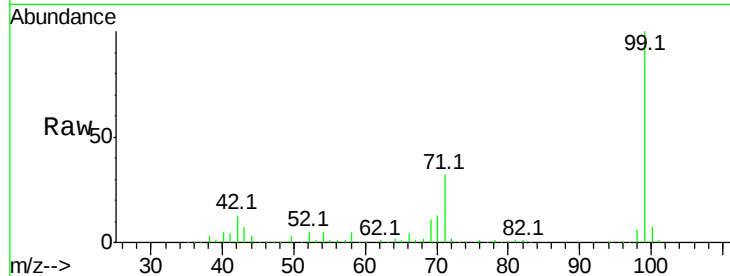

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

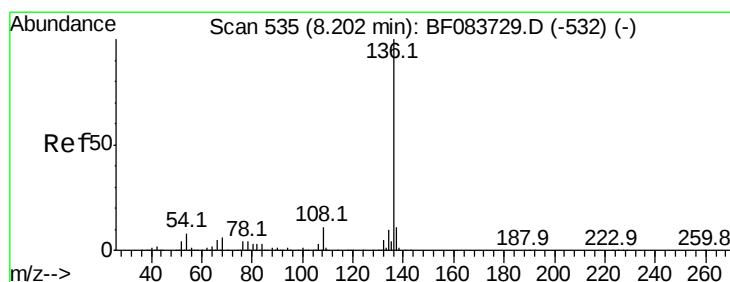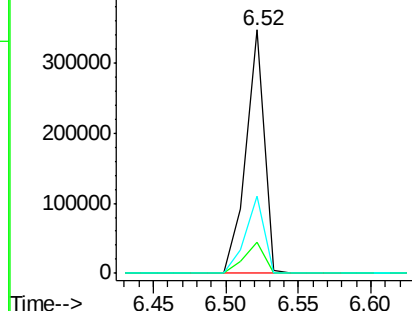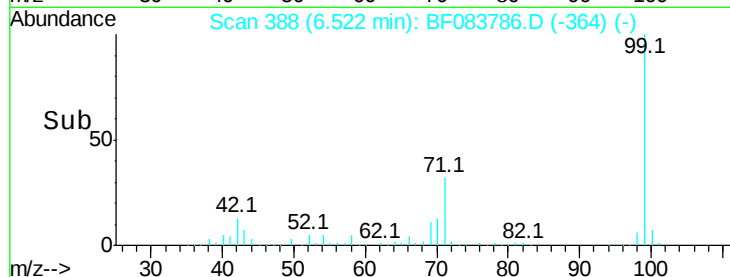

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.18 min Scan# 533

Delta R.T. -0.03 min

Lab File: BF083786.D

Acq: 14 Dec 2015 23:19

Tgt Ion: 136 Resp: 404379


Ion Ratio Lower Upper

136 100

137 11.3 8.7 13.1

54 8.4 7.8 11.6

68 6.6 5.7 8.5


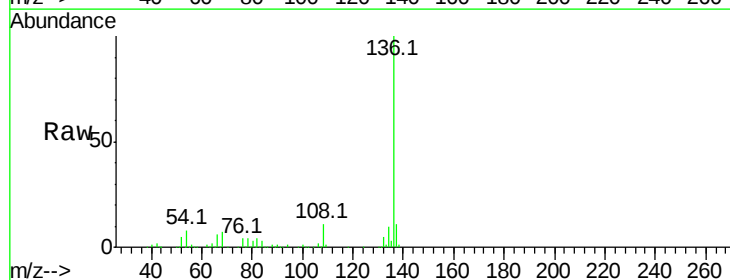



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0



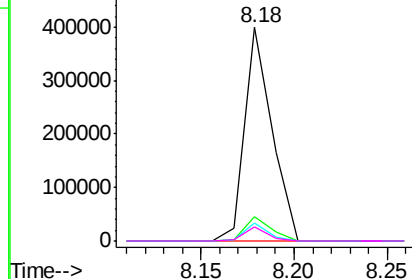
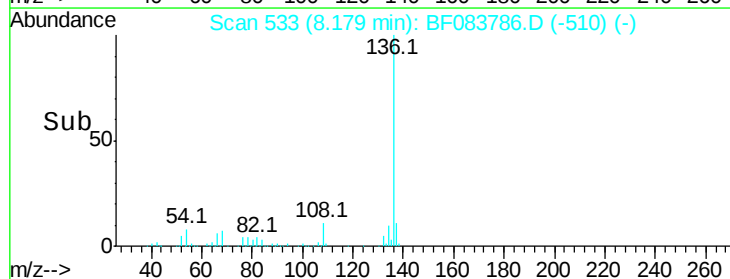


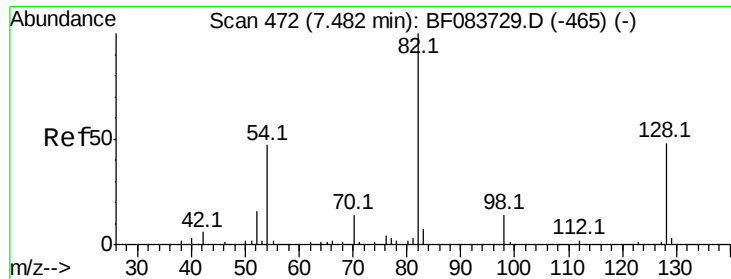

#23
 Nitrobenzene-d5
 Concen: 80.97 ng
 RT: 7.46 min Scan# 470
 Delta R.T. -0.02 min
 Lab File: BF083786.D
 Acq: 14 Dec 2015 23:19




Instrument :
 BNA_F
 ClientSampleId :
 W-35


Tot Ion: 82 Resp: 585278
 Ion Ratio Lower Upper
 82 100
 128 47.4 30.7 46.1#
 54 46.1 42.5 63.7

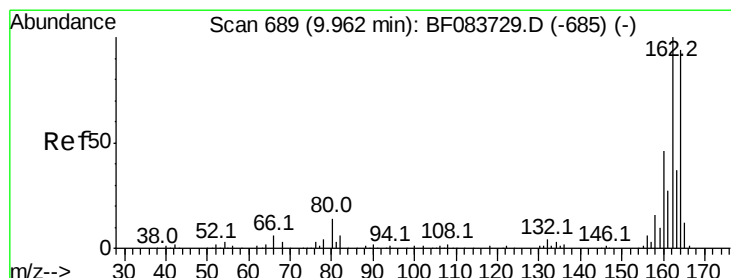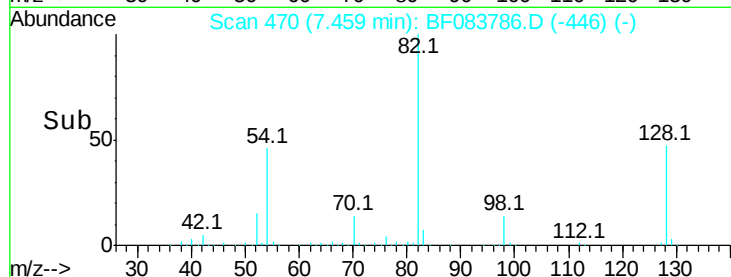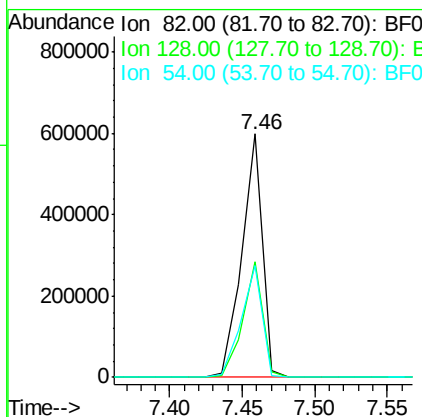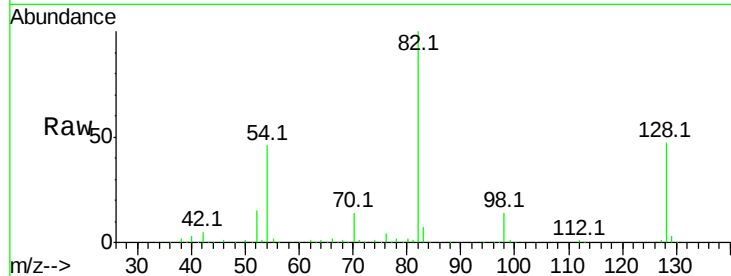

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.94 min Scan# 687
 Delta R.T. -0.02 min
 Lab File: BF083786.D
 Acq: 14 Dec 2015 23:19

Tgt Ion: 164 Resp: 216029
 Ion Ratio Lower Upper
 164 100
 162 103.4 78.8 118.2
 160 47.2 33.4 50.2

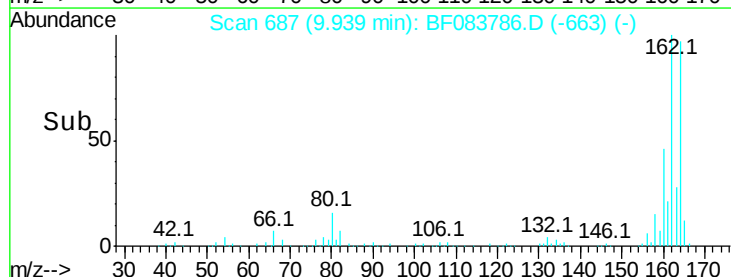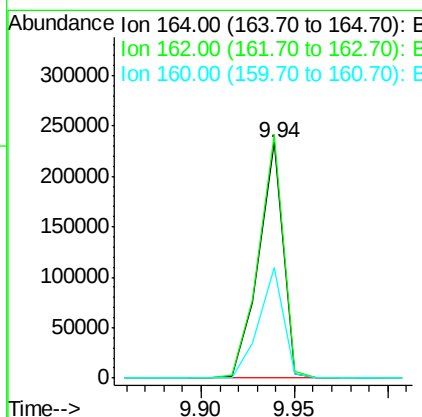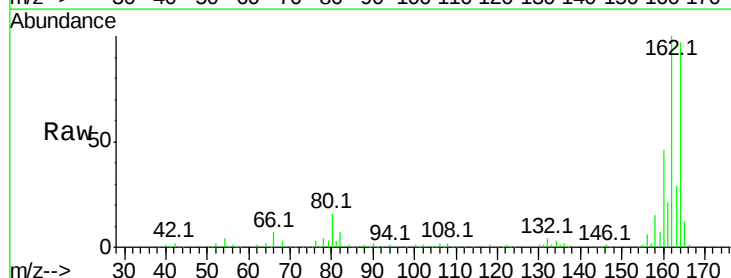


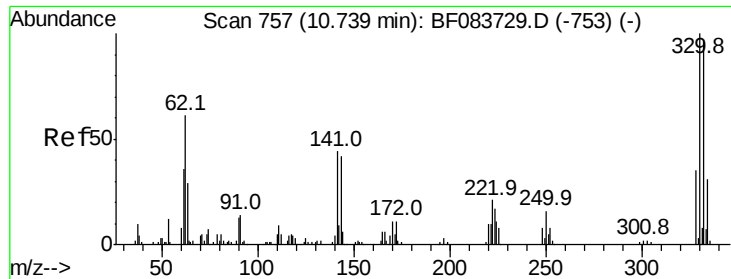




#41
 2,4,6-Tribromophenol
 Concen: 142.78 ng
 RT: 10.73 min Scan# 756
 Delta R.T. -0.02 min
 Lab File: BF083786.D
 Acq: 14 Dec 2015 23:19

Instrument :
 BNA_F
 ClientSampleId :
 W-35

Tot Ion:330 Resp: 314308
 Ion Ratio Lower Upper
 330 100
 332 96.2 0.0 0.0#
 141 30.4 0.0 0.0#

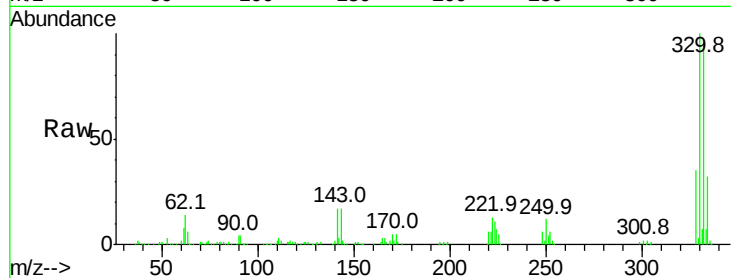


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

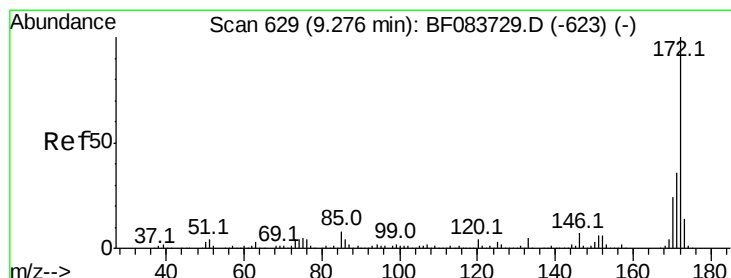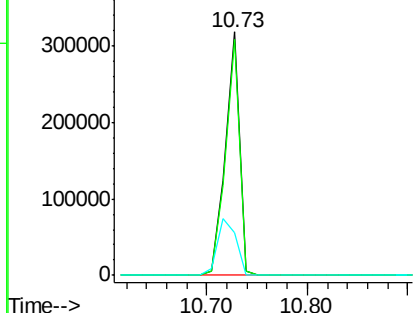
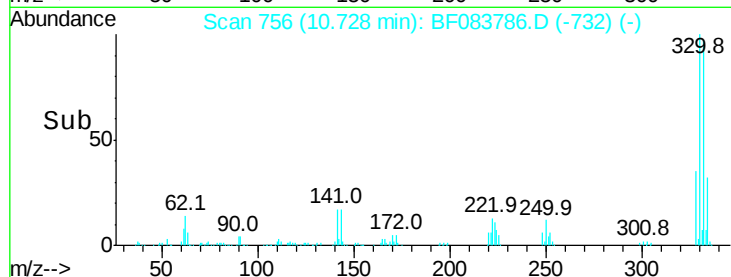



#44
 2-Fluorobiphenyl
 Concen: 79.60 ng
 RT: 9.26 min Scan# 628
 Delta R.T. -0.02 min
 Lab File: BF083786.D
 Acq: 14 Dec 2015 23:19

Tgt Ion:172 Resp: 1196575
 Ion Ratio Lower Upper
 172 100
 171 37.4 28.6 42.8
 170 24.3 19.4 29.0

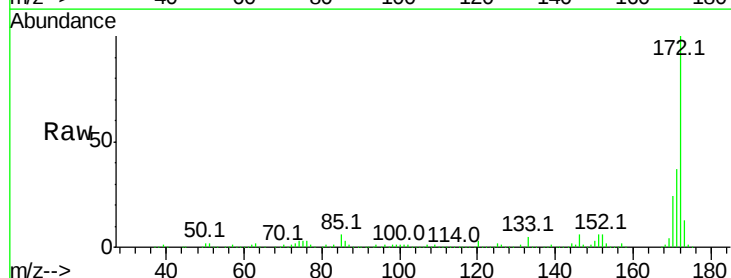

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

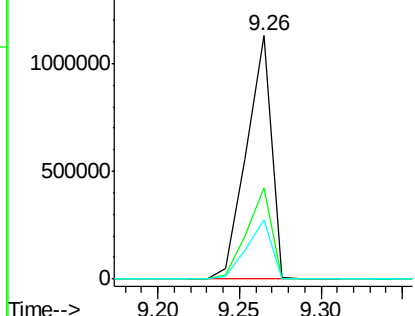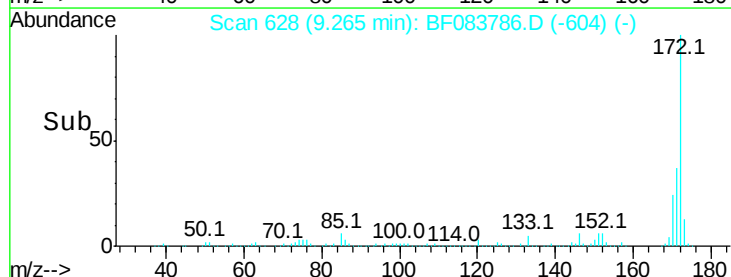


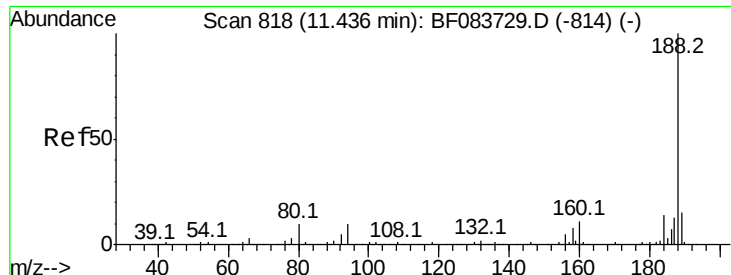




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.41 min Scan# 816
Delta R.T. -0.03 min
Lab File: BF083786.D
Acq: 14 Dec 2015 23:19

Instrument :
BNA_F
ClientSampled :
W-35

Tot Ion:188 Resp: 368430
Ion Ratio Lower Upper
188 100
94 13.1 9.4 14.2
80 14.1 10.6 16.0

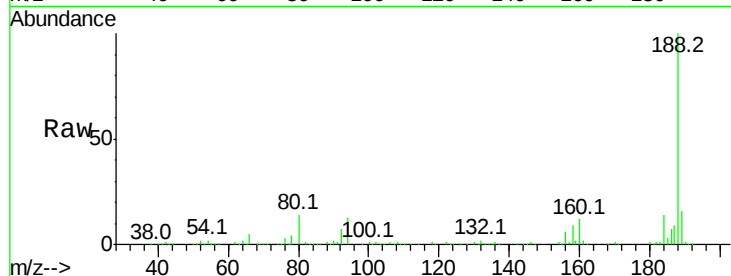


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

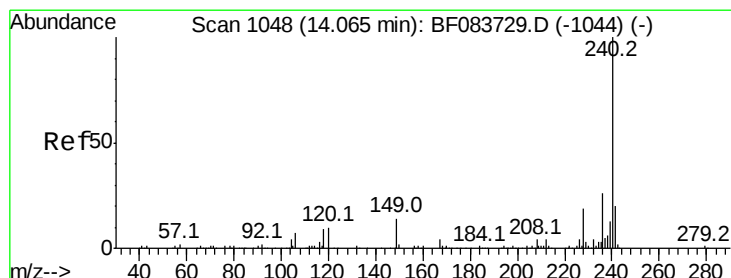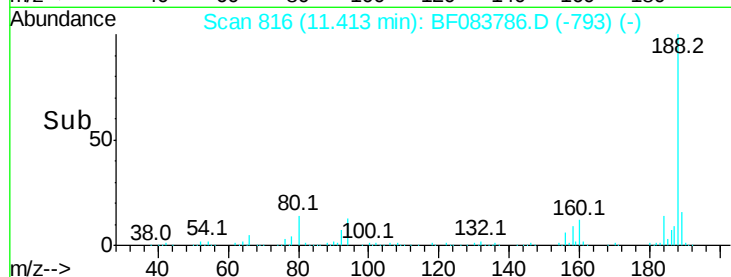
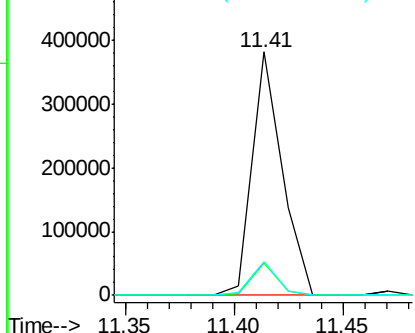



#75
Chrysene-d12
Concen: 20.00 ng
RT: 14.04 min Scan# 1046
Delta R.T. -0.03 min
Lab File: BF083786.D
Acq: 14 Dec 2015 23:19

Tgt Ion:240 Resp: 303333
Ion Ratio Lower Upper
240 100
120 17.3 8.1 12.1#
236 25.6 20.8 31.2

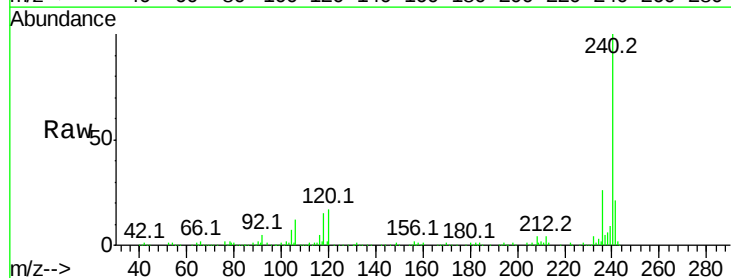

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

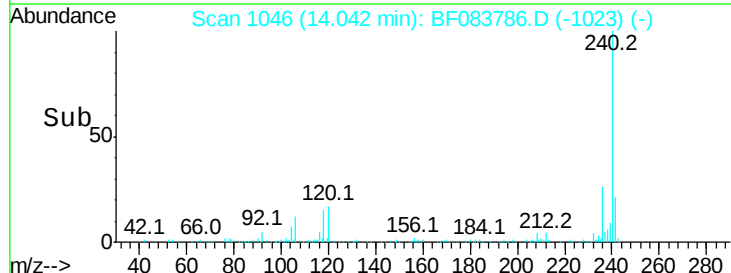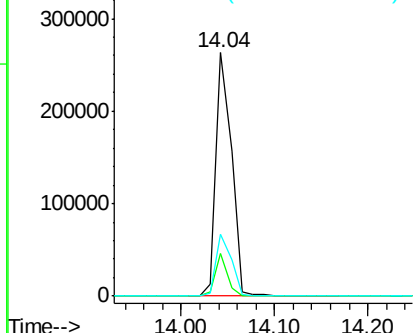


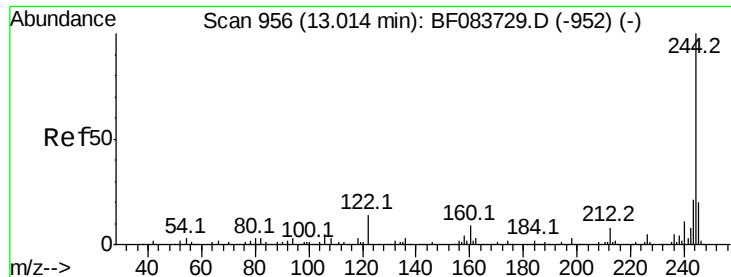




#78
 Terphenyl-d14
 Concen: 70.38 ng
 RT: 13.00 min Scan# 955
 Delta R.T. -0.02 min
 Lab File: BF083786.D
 Acq: 14 Dec 2015 23:19

Instrument :
 BNA_F
 ClientSampled :
 W-35

Tot Ion:244 Resp: 992451
 Ion Ratio Lower Upper
 244 100
 212 7.6 6.1 9.1
 122 13.3 11.0 16.6

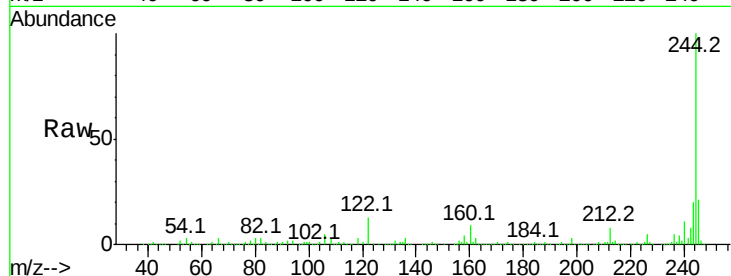


Abundance Ion 244.00 (243.70 to 244.70): E
 Ion 212.00 (211.70 to 212.70): E
 Ion 122.00 (121.70 to 122.70): E

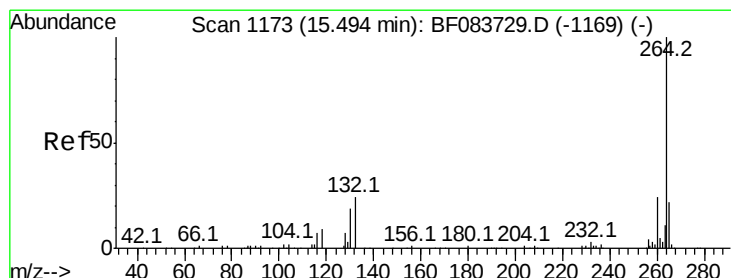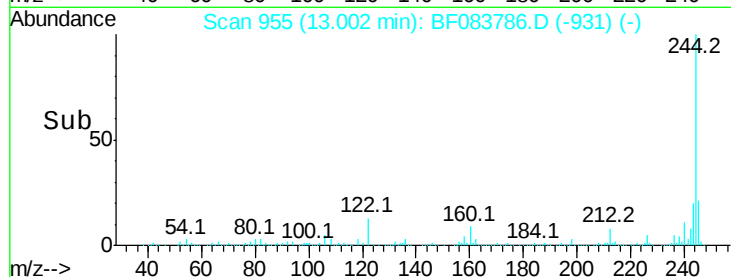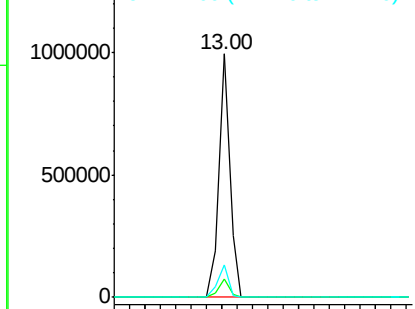

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.48 min Scan# 1172
 Delta R.T. -0.02 min
 Lab File: BF083786.D
 Acq: 14 Dec 2015 23:19

Tgt Ion:264 Resp: 227440
 Ion Ratio Lower Upper
 264 100
 260 23.8 19.4 29.0
 265 21.3 17.8 26.6

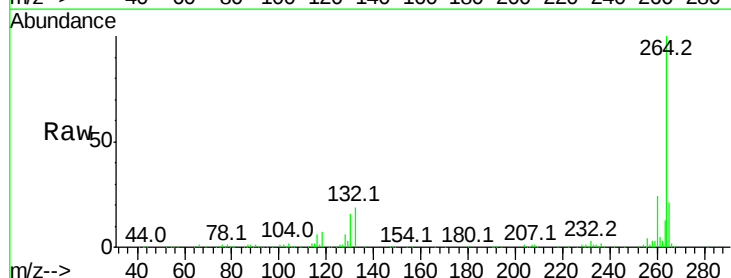

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

