

Data Path : Z:\HPCHEM1\BNA F\DATA\BF121415\
 Data File : BF083791.D
 Acq On : 15 Dec 2015 1:40
 Operator : UM/IZ
 Sample : G4779-06
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 W-41

Quant Time: Dec 15 03:38:07 2015
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121315.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 14 01:30:12 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.90	152	119375	20.00	ng	-0.02
21) Naphthalene-d8	8.18	136	438846	20.00	ng	-0.03
38) Acenaphthene-d10	9.94	164	227157	20.00	ng	-0.02
63) Phenanthrene-d10	11.41	188	393015	20.00	ng	-0.03
75) Chrysene-d12	14.04	240	346454	20.00	ng	-0.03
86) Perylene-d12	15.48	264	270409	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.50	112	391041	52.85	ng	-0.02
7) Phenol-d6	6.52	99	330885	35.31	ng	-0.02
23) Nitrobenzene-d5	7.46	82	588187	74.99	ng	-0.02
41) 2,4,6-Tribromophenol	10.73	330	292577	126.40	ng	-0.02
44) 2-Fluorobiphenyl	9.26	172	1218460	76.16	ng	-0.02
78) Terphenyl-d14	13.00	244	1190696	73.93	ng	-0.02
Target Compounds						
49) Dimethylphthalate	9.65	163	37413	2.11	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF121415\
Data File : BF083791.D
Acq On : 15 Dec 2015 1:40
Operator : UM/IZ
Sample : G4779-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
W-41

Quant Time: Dec 15 03:38:07 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 14 01:30:12 2015
Response via : Initial Calibration

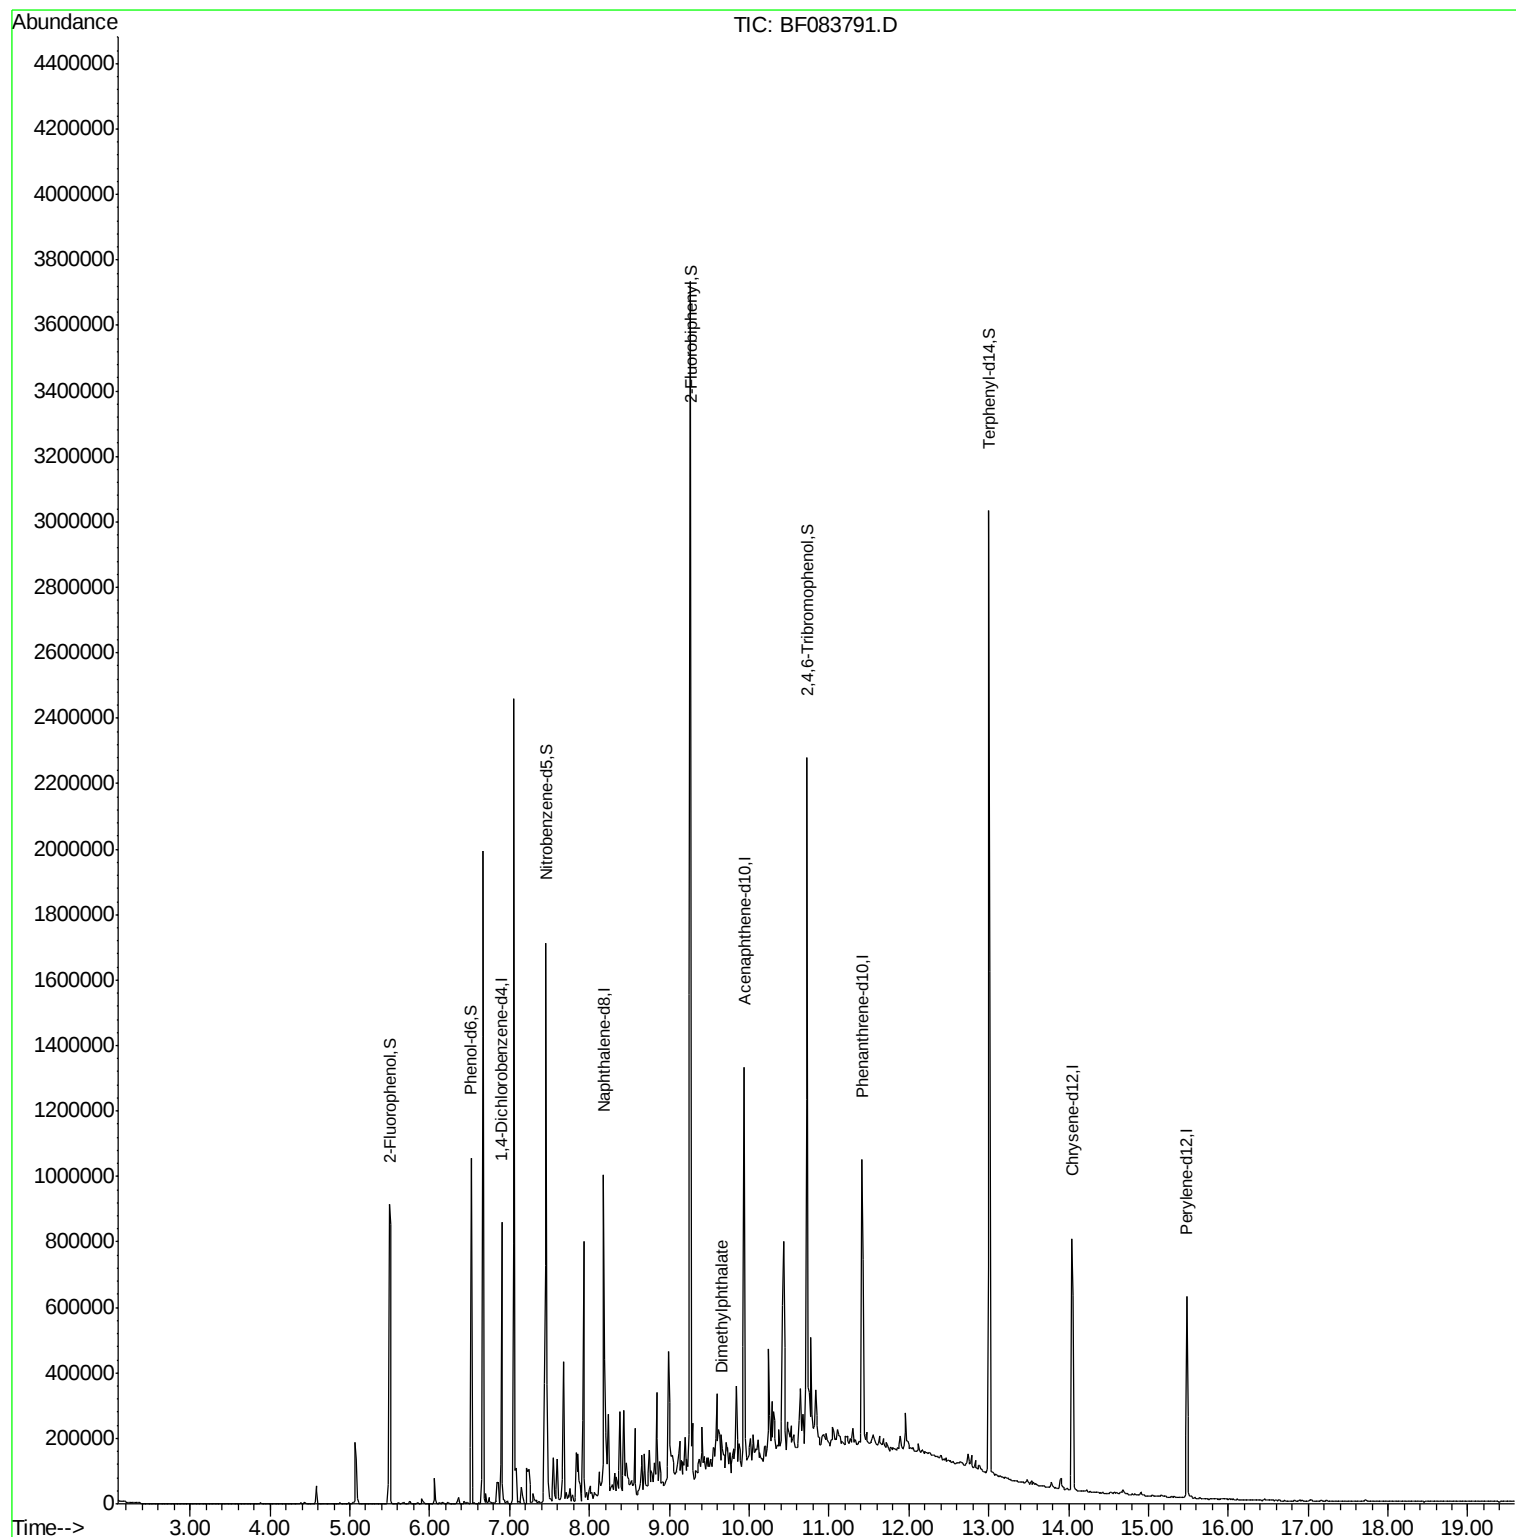

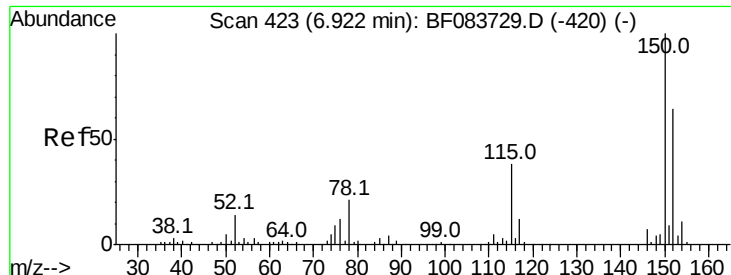

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.90 min Scan# 421

Delta R.T. -0.02 min

Lab File: BF083791.D

Acq: 15 Dec 2015 1:40

Instrument :

BNA_F

ClientSampleId :

W-41


Tot Ion:152 Resp: 119375

Ion Ratio Lower Upper

152 100

150 155.2 126.5 189.7




115 63.7 52.3 78.5

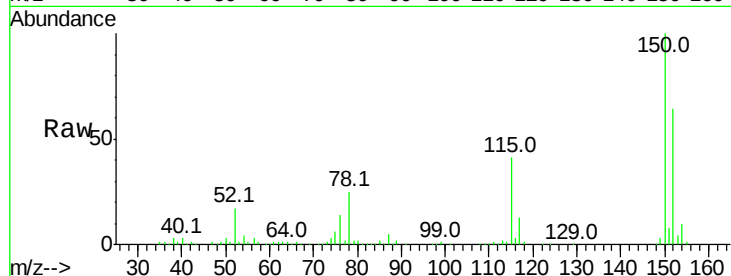

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

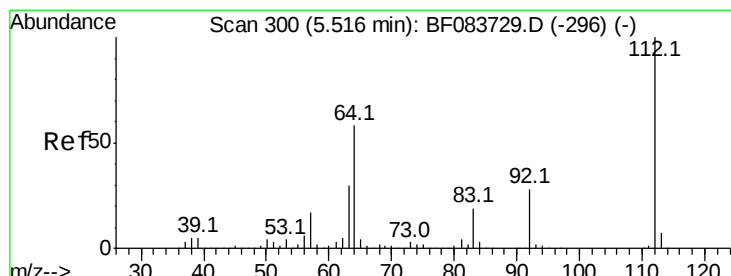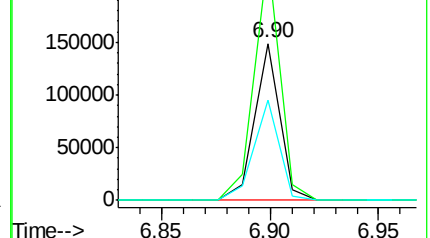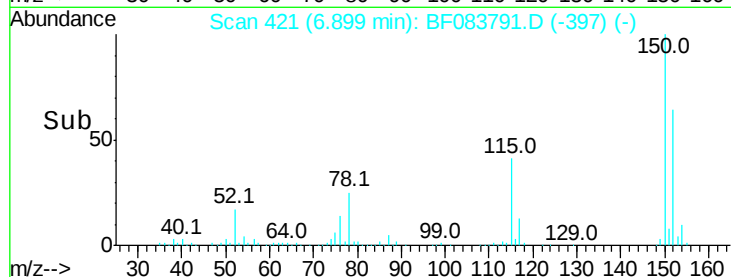

#5

2-Fluorophenol

Concen: 52.85 ng

RT: 5.50 min Scan# 299

Delta R.T. -0.02 min

Lab File: BF083791.D

Acq: 15 Dec 2015 1:40


Tgt Ion:112 Resp: 391041

Ion Ratio Lower Upper

112 100

64 43.0 50.5 75.7#



63 21.6 25.8 38.6#

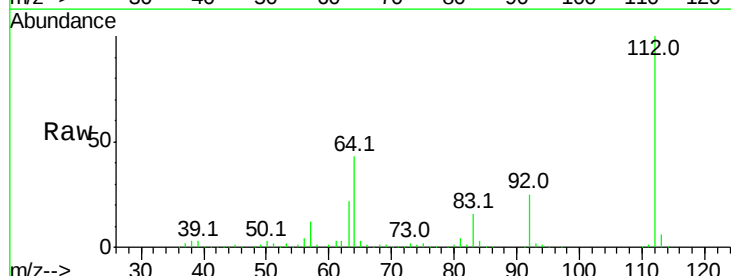


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

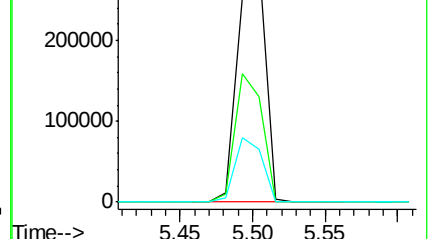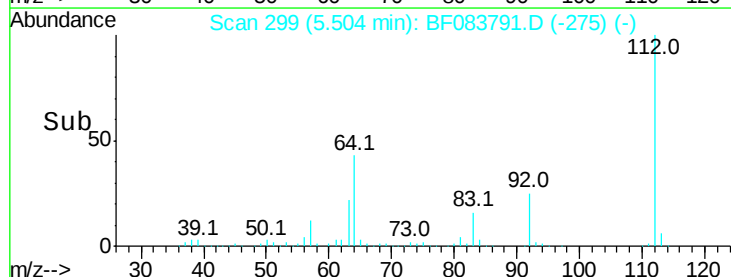

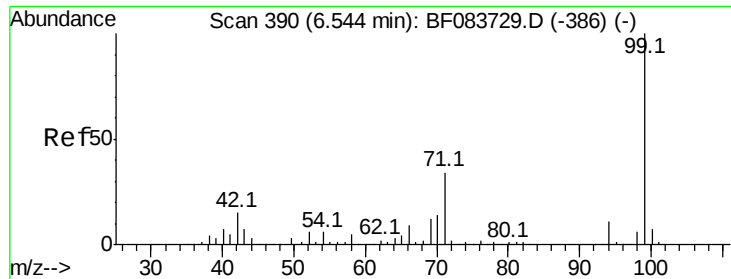

#7

Phenol-d6

Concen: 35.31 ng

RT: 6.52 min Scan# 388

Delta R.T. -0.02 min

Lab File: BF083791.D

Acq: 15 Dec 2015 1:40

Instrument :

BNA_F

ClientSampled :

W-41


Tot Ion: 99 Resp: 330885

Ion Ratio Lower Upper

99 100

42 15.3 17.3 25.9#




71 34.7 26.6 40.0

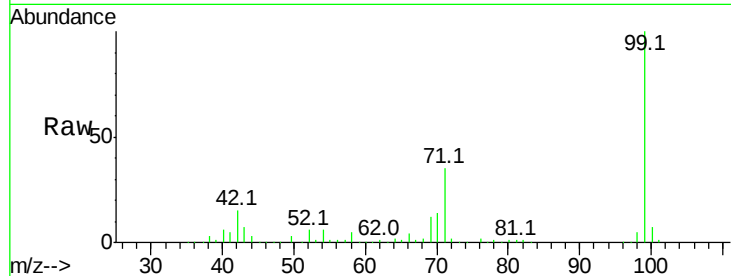

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

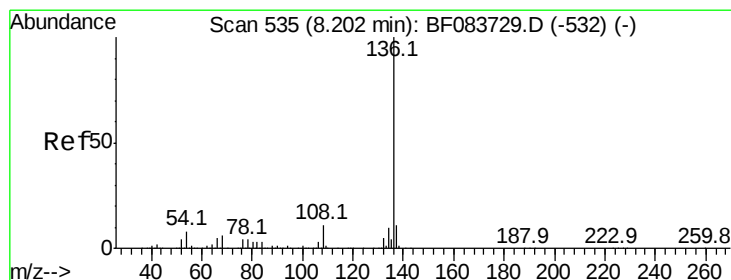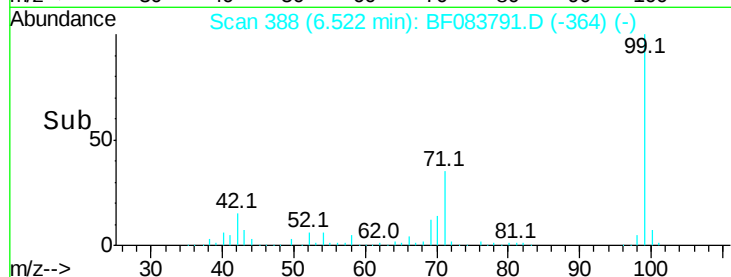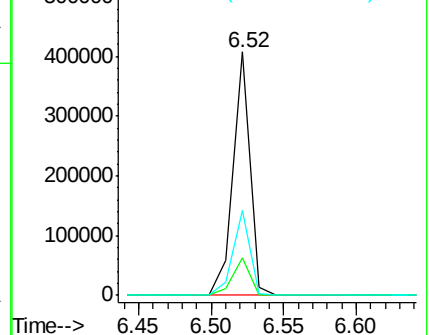

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.18 min Scan# 533

Delta R.T. -0.03 min

Lab File: BF083791.D

Acq: 15 Dec 2015 1:40

Tgt Ion: 136 Resp: 438846


Ion Ratio Lower Upper

136 100

137 11.4 8.7 13.1

54 8.6 7.8 11.6

68 6.5 5.7 8.5


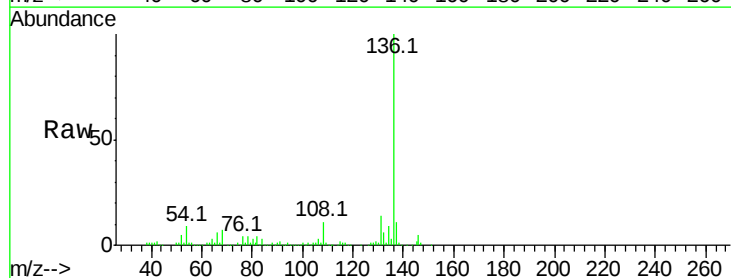



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0



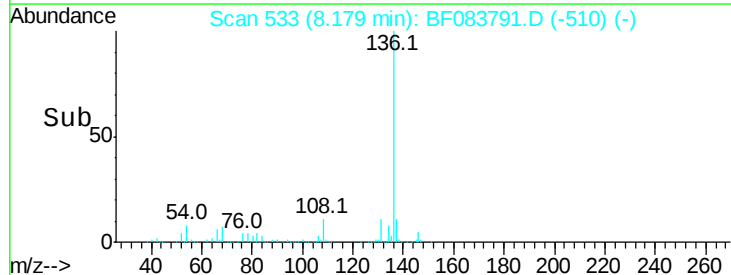
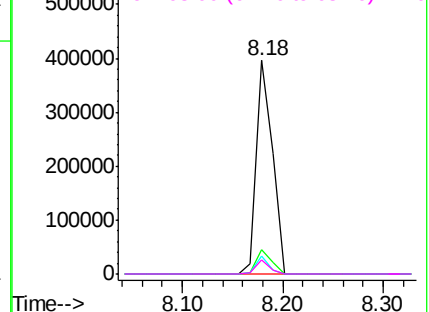


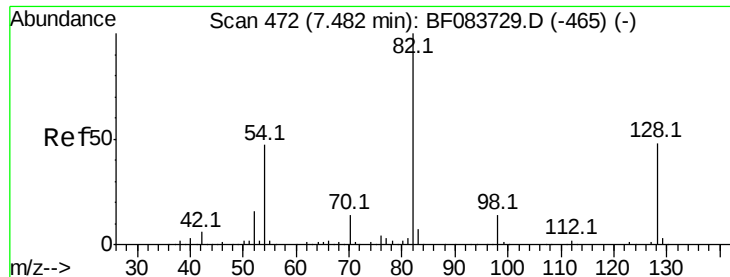

#23
 Nitrobenzene-d5
 Concen: 74.99 ng
 RT: 7.46 min Scan# 470
 Delta R.T. -0.02 min
 Lab File: BF083791.D
 Acq: 15 Dec 2015 1:40




Instrument :
 BNA_F
 ClientSampled :
 W-41


Tot Ion: 82 Resp: 588187
 Ion Ratio Lower Upper
 82 100
 128 46.2 30.7 46.1#
 54 46.8 42.5 63.7

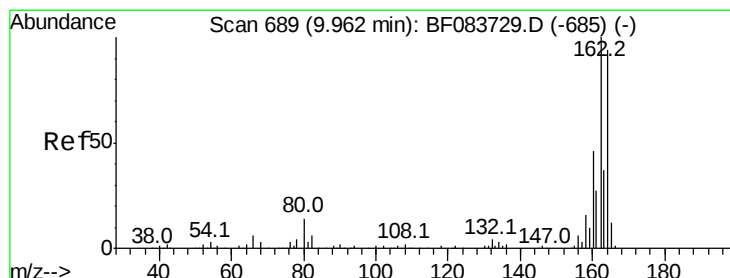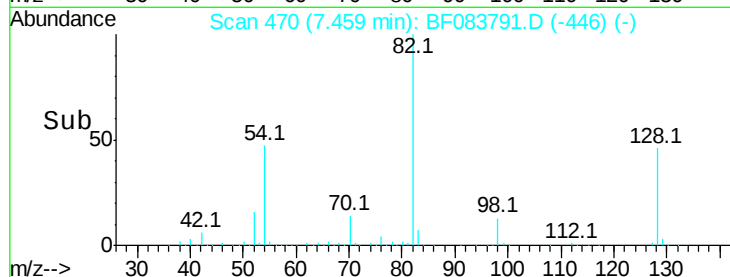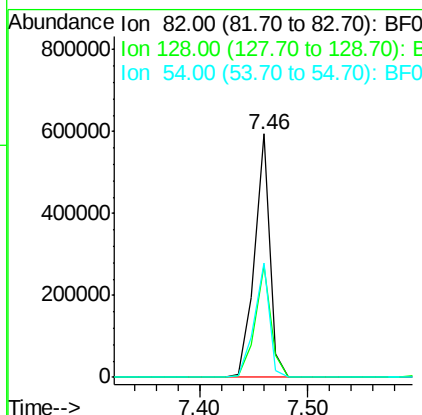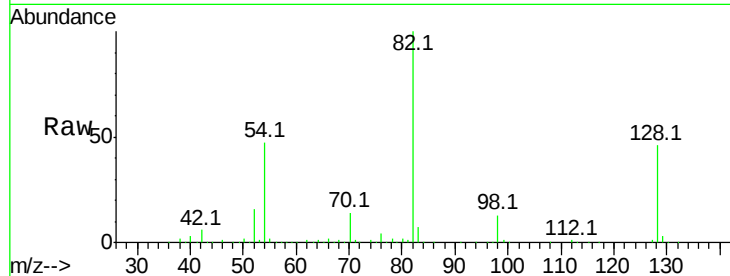

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.94 min Scan# 687
 Delta R.T. -0.02 min
 Lab File: BF083791.D
 Acq: 15 Dec 2015 1:40

Tgt Ion: 164 Resp: 227157
 Ion Ratio Lower Upper
 164 100
 162 104.2 78.8 118.2
 160 50.2 33.4 50.2#

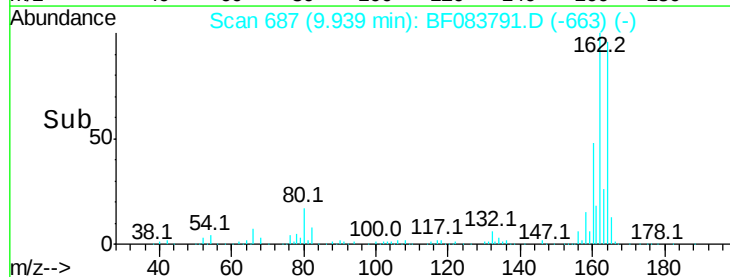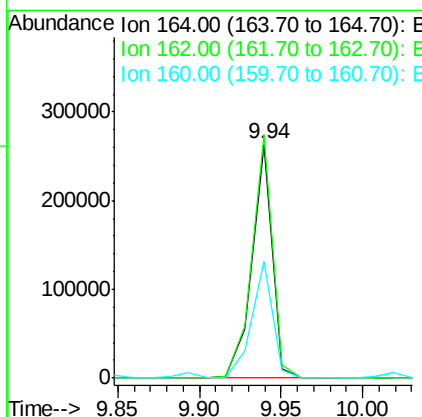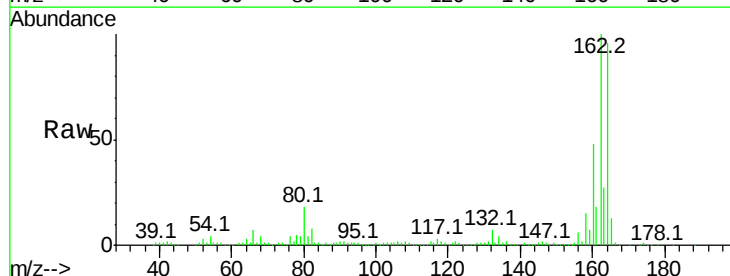


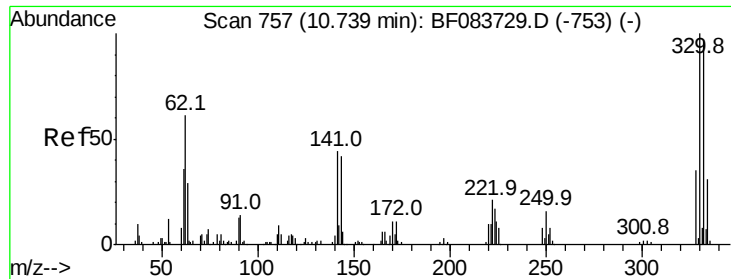




#41
 2,4,6-Tribromophenol
 Concen: 126.40 ng
 RT: 10.73 min Scan# 756
 Delta R.T. -0.02 min
 Lab File: BF083791.D
 Acq: 15 Dec 2015 1:40

Instrument :
 BNA_F
 ClientSampleId :
 W-41

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.1	0.0	0.0#
141	37.7	0.0	0.0#

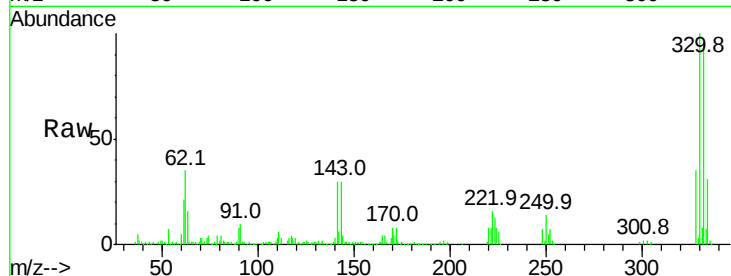


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

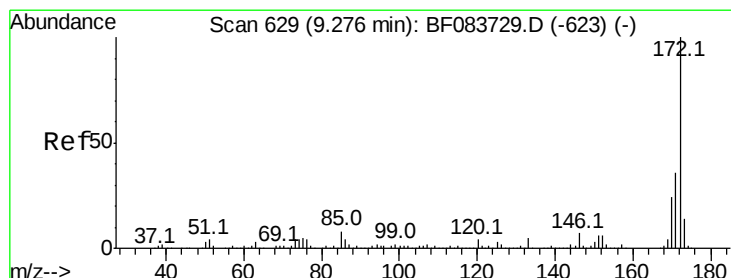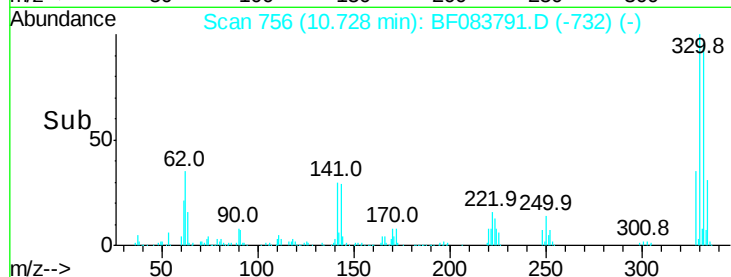
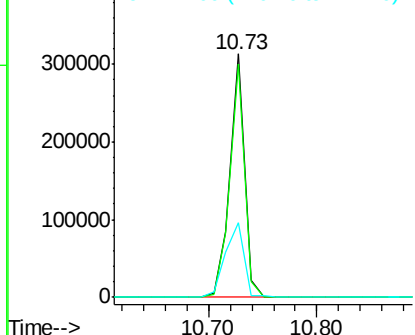



#44
 2-Fluorobiphenyl
 Concen: 76.16 ng
 RT: 9.26 min Scan# 628
 Delta R.T. -0.02 min
 Lab File: BF083791.D
 Acq: 15 Dec 2015 1:40

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.5	28.6	42.8
170	25.0	19.4	29.0

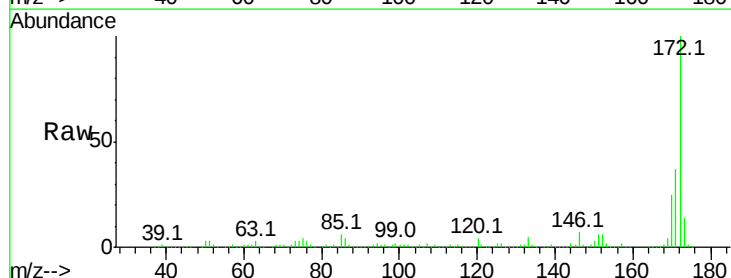

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

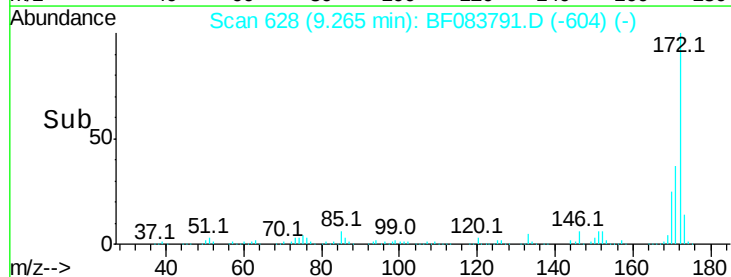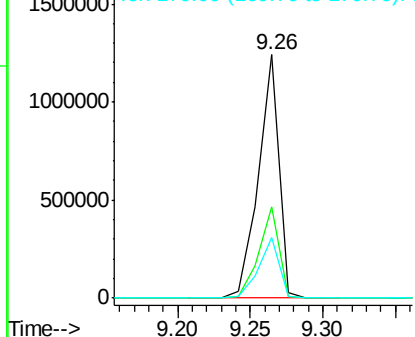


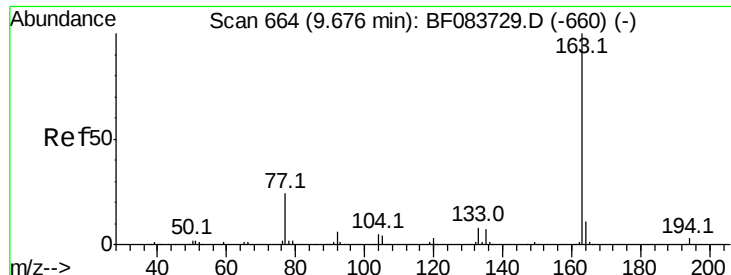




#49
Dimethylphthalate
Concen: 2.11 ng
RT: 9.65 min Scan# 662
Delta R.T. -0.03 min
Lab File: BF083791.D
Acq: 15 Dec 2015 1:40

Instrument :
BNA_F
ClientSampleId :
W-41

Tot Ion:163 Resp: 37413
Ion Ratio Lower Upper
163 100
194 3.9 2.8 4.2
164 10.5 8.6 13.0

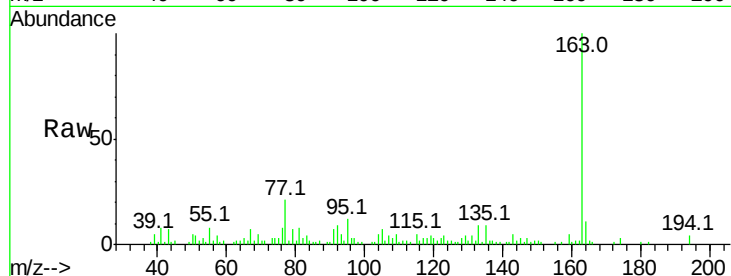


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

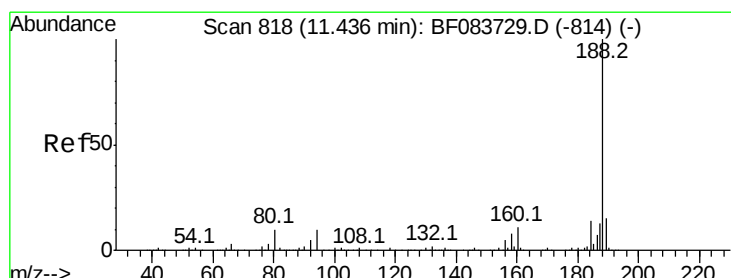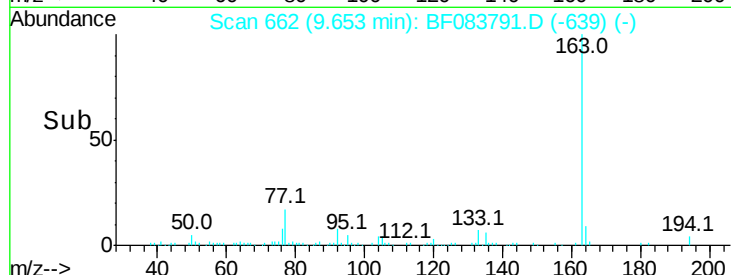
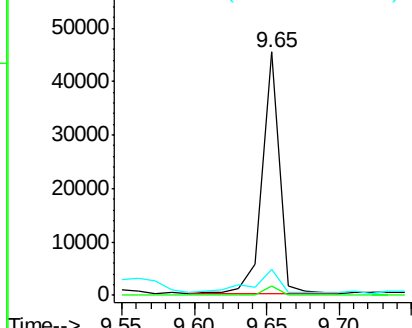



#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.41 min Scan# 816
Delta R.T. -0.03 min
Lab File: BF083791.D
Acq: 15 Dec 2015 1:40

Tgt Ion:188 Resp: 393015
Ion Ratio Lower Upper
188 100
94 13.5 9.4 14.2
80 15.0 10.6 16.0

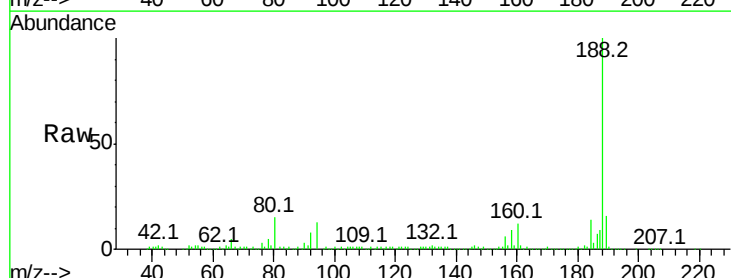

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

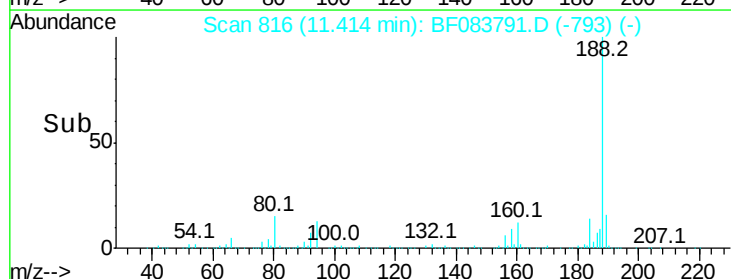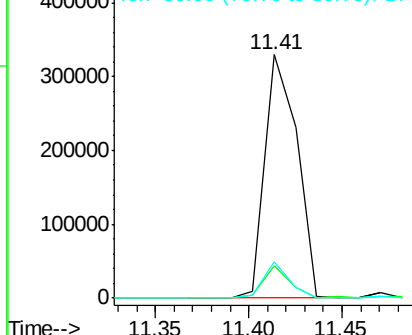

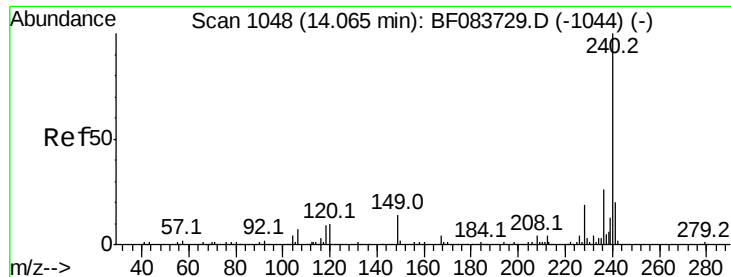

#75

Chrysene-d12

Concen: 20.00 ng

RT: 14.04 min Scan# 1046

Delta R.T. -0.03 min

Lab File: BF083791.D

Acq: 15 Dec 2015 1:40

Instrument :

BNA_F

ClientSampleId :

W-41


Tot Ion:240 Resp: 346454

Ion Ratio Lower Upper

240 100

120 18.8 8.1 12.1#




236 25.7 20.8 31.2

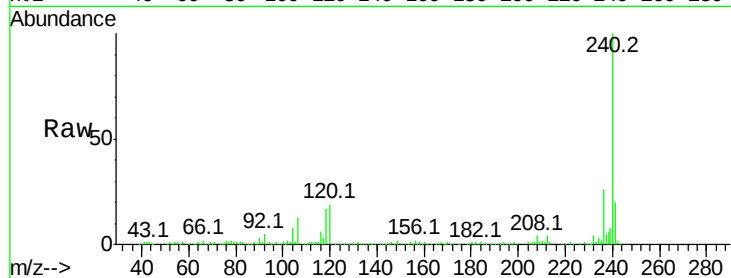

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

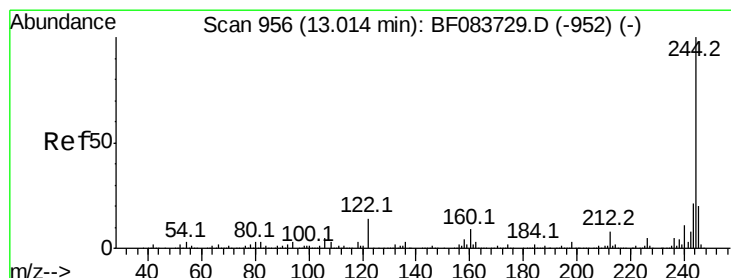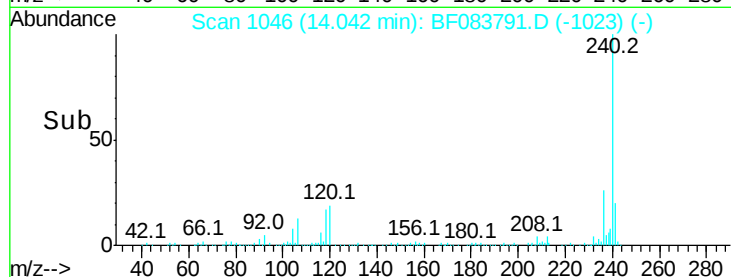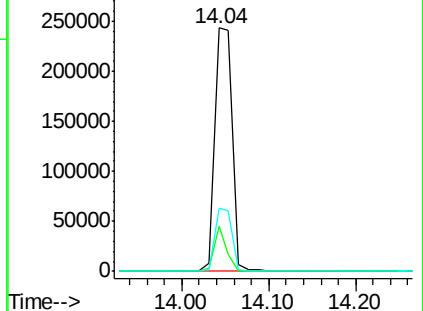

#78

Terphenyl-d14

Concen: 73.93 ng

RT: 13.00 min Scan# 955

Delta R.T. -0.02 min

Lab File: BF083791.D

Acq: 15 Dec 2015 1:40


Tgt Ion:244 Resp: 1190696

Ion Ratio Lower Upper

244 100

212 7.7 6.1 9.1



122 14.1 11.0 16.6

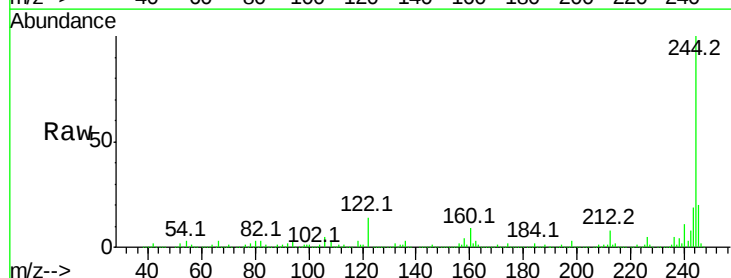


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

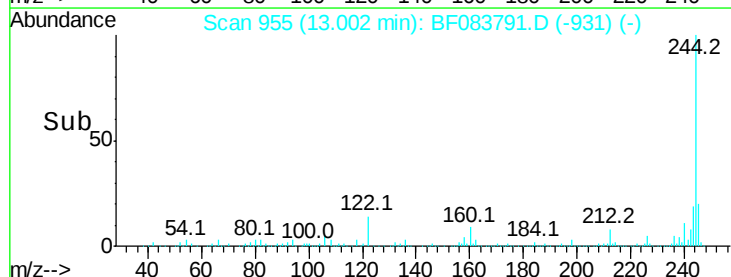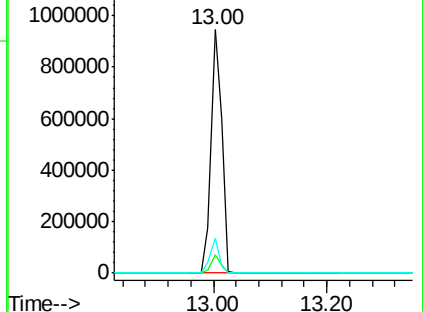


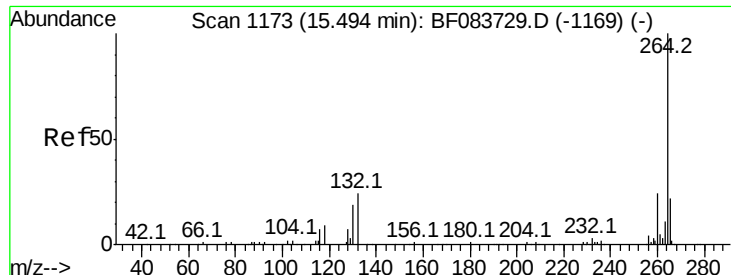

#86
 Pervlene-d12
 Concen: 20.00 ng
 RT: 15.48 min Scan# 1172
 Delta R.T. -0.02 min
 Lab File: BF083791.D
 Acq: 15 Dec 2015 1:40

Instrument :
 BNA_F
 ClientSampleId :
 W-41

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.4	19.4	29.0
265	21.6	17.8	26.6

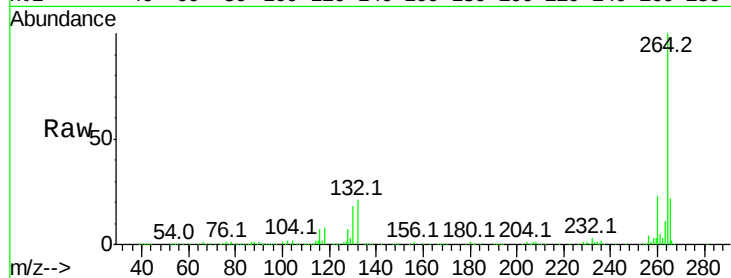

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

