


Data Path : Z:\HPCHEM1\BNA F\Data\BF121415\
 Data File : BF083775.D
 Acq On : 14 Dec 2015 18:08
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 14 01:30:12 2015

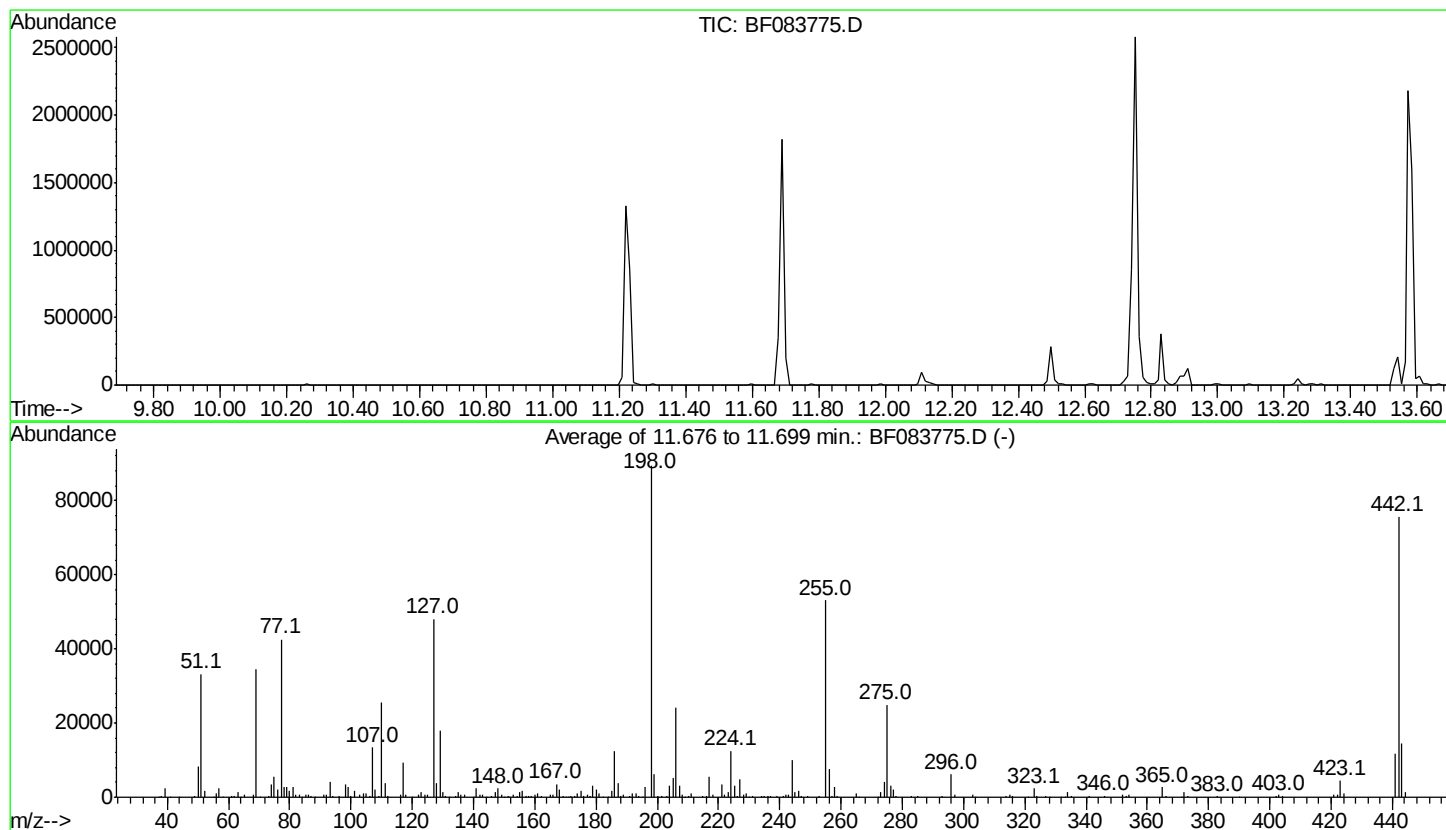

AutoFind: Scans 839, 840, 841; Background Corrected with Scan 836

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.2	33284	PASS
68	69	0.00	2	1.9	651	PASS
69	198	0.00	100	38.7	34635	PASS
70	69	0.00	2	0.4	131	PASS
127	198	10	80	53.8	48103	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	89414	PASS
199	198	5	9	6.9	6167	PASS
275	198	10	60	27.9	24988	PASS
365	198	1	100	3.0	2666	PASS
441	442	0.01	24	15.3	11601	PASS
442	198	50	100	84.7	75730	PASS
443	442	15	24	19.0	14423	PASS