
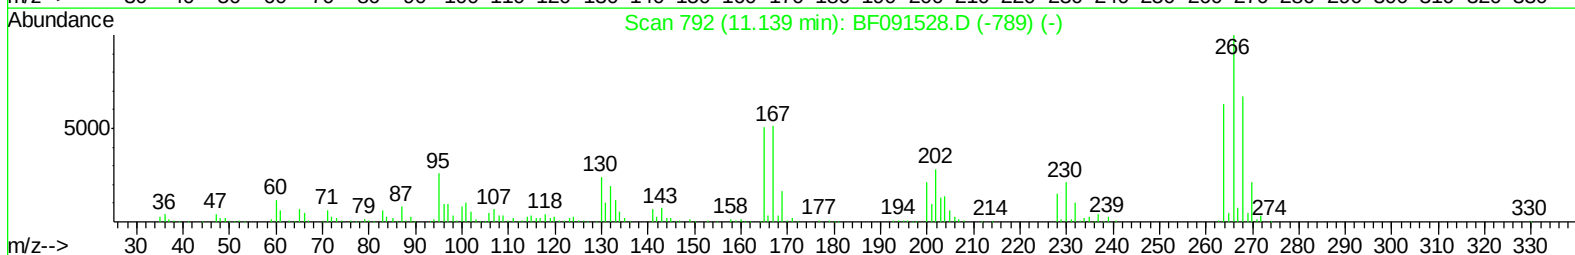
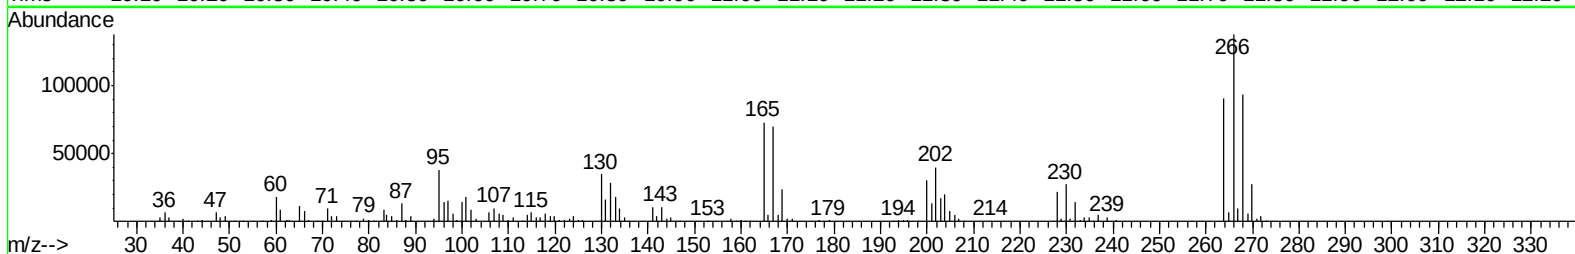


Data Path : Z:\HPCHEM1\BNA_F\Data\BF121416\
Data File : BF091586.D
Acq On : 14 Dec 2016 16:10
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 19 04:41:53 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF120916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 16 00:35:41 2016
Response via : Initial Calibration

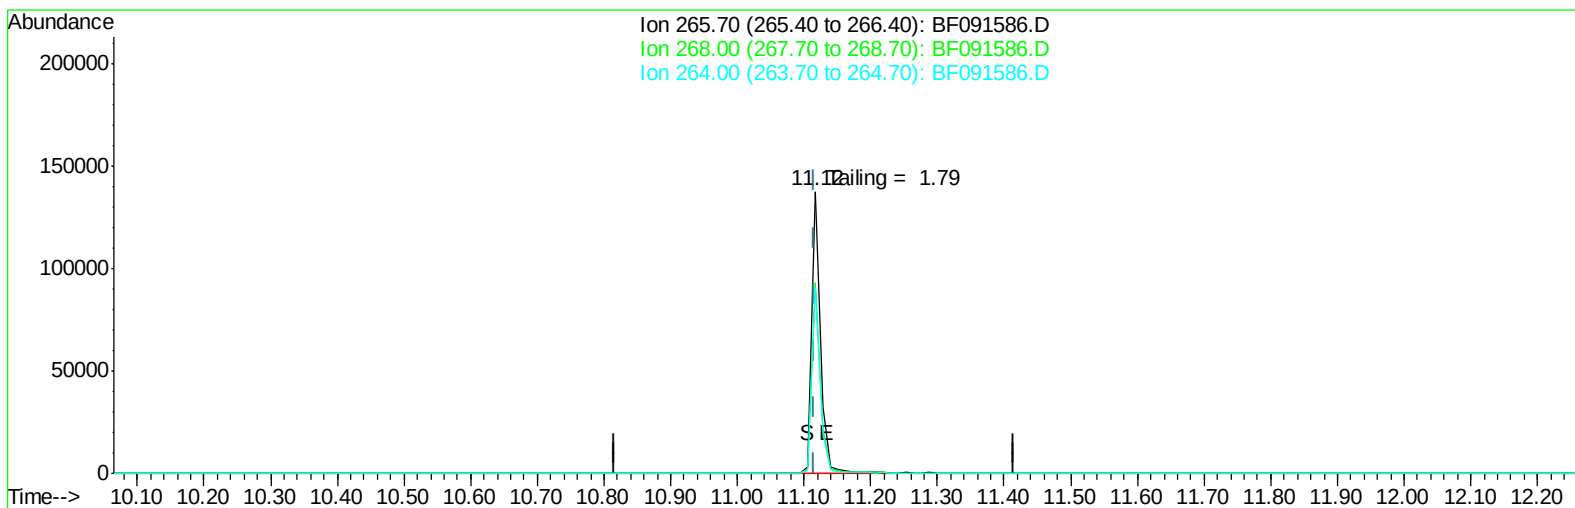

TIC: BF091586.D

(69) Pentachlorophenol (C)




11.116min (-0.000) 54779.69ng

response 126534

Ion	Exp%	Act%
265.70	100	100
268.00	62.90	67.74
264.00	60.20	65.94
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF121416\
Data File : BF091586.D
Acq On : 14 Dec 2016 16:10
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 19 04:41:53 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF120916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 16 00:35:41 2016
Response via : Initial Calibration

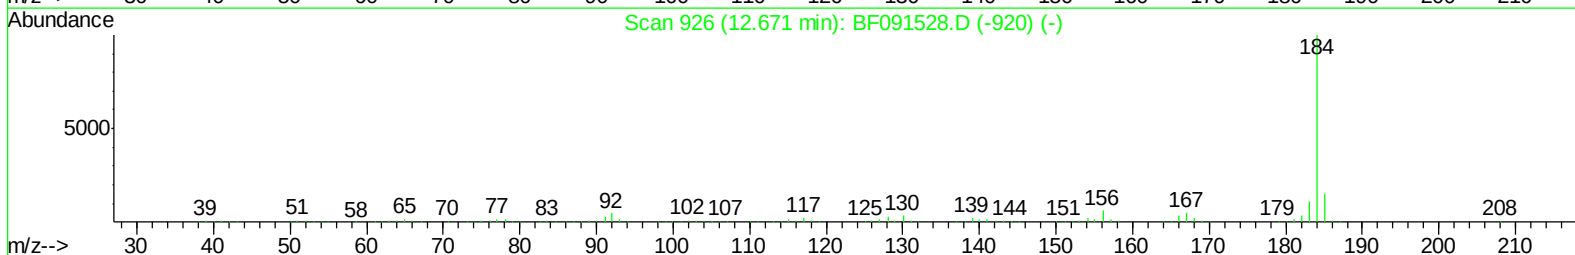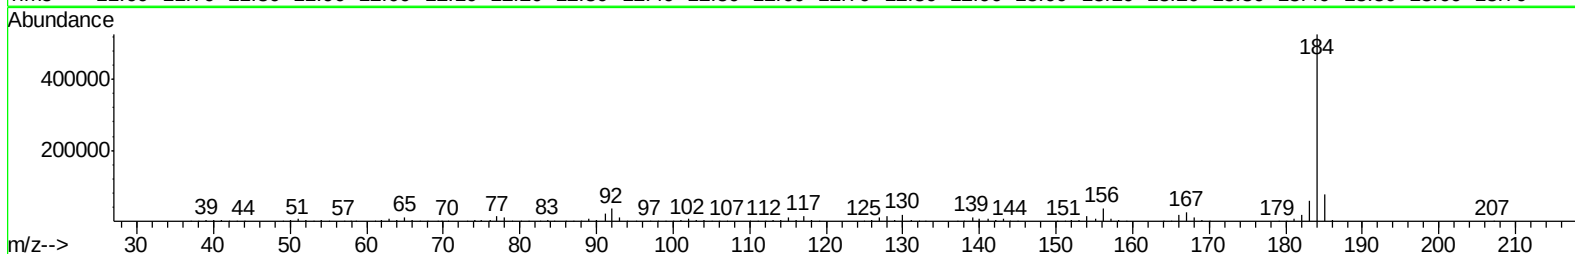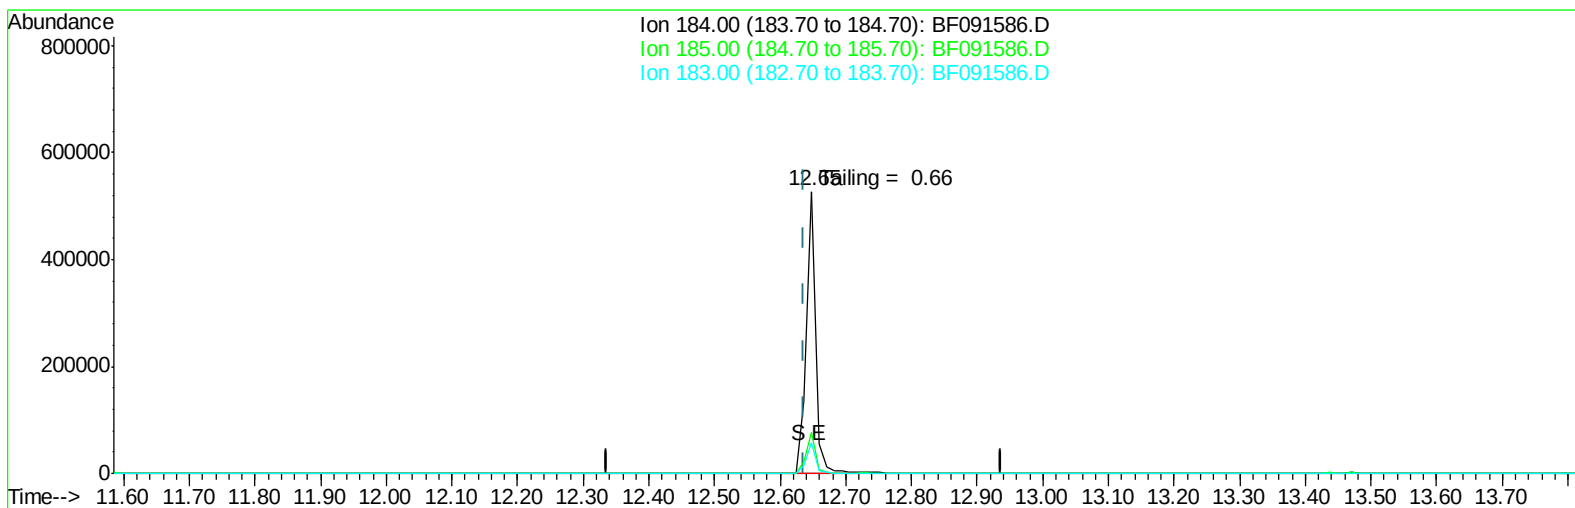

TIC: BF091586.D

(76) Benzidine

12.648min (+0.011) 4267.64ng

response 517402

Ion	Exp%	Act%
184.00	100	100
185.00	16.40	14.44
183.00	11.10	10.97
0.00	0.00	0.00