
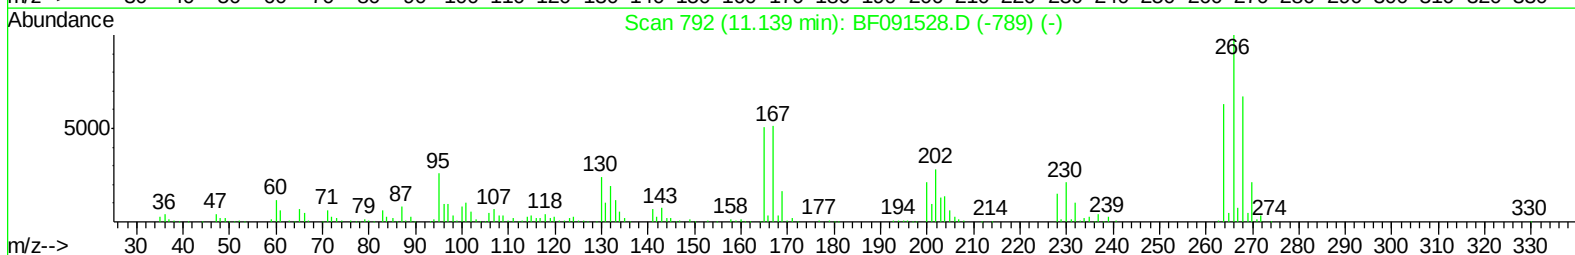
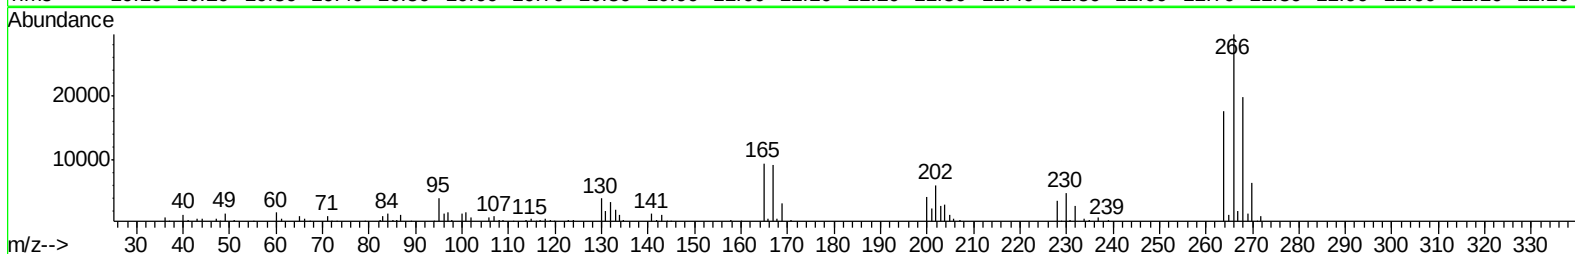


Data Path : Z:\HPCHEM1\BNA_F\Data\BF121416\
Data File : BF091611.D
Acq On : 15 Dec 2016 5:46
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 19 04:42:41 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF120916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 16 00:35:41 2016
Response via : Initial Calibration

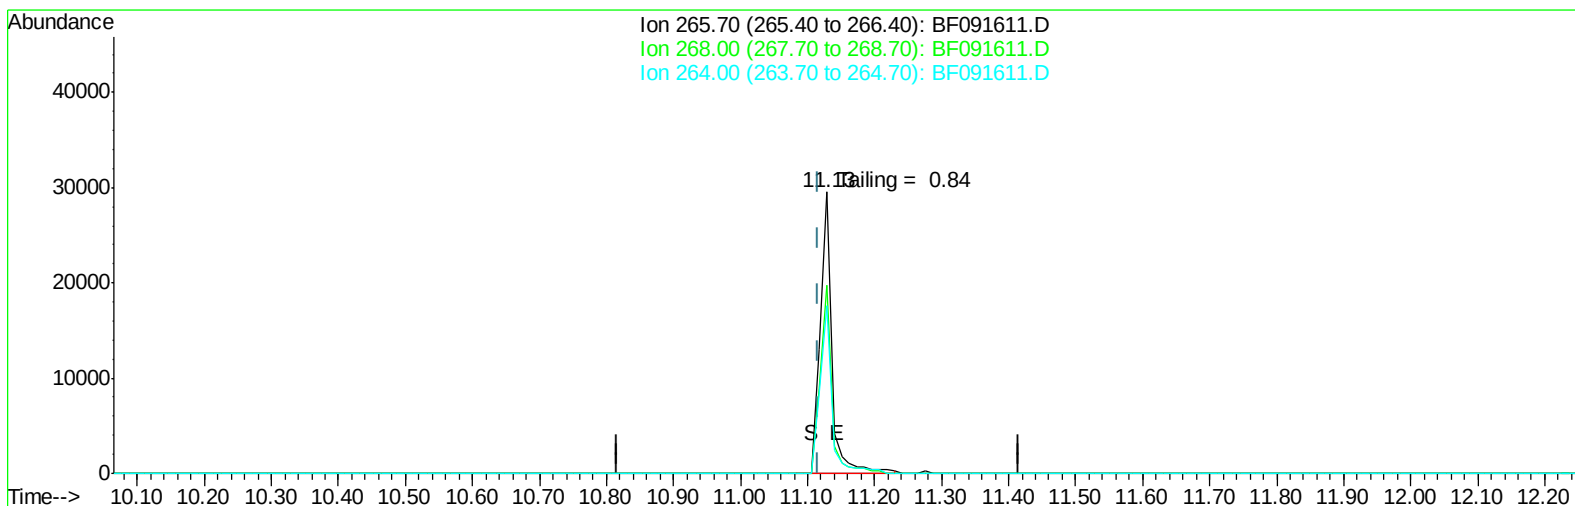

TIC: BF091611.D

(69) Pentachlorophenol (C)




11.128min (+0.012) 15656.67ng

response 35977

Ion	Exp%	Act%
265.70	100	100
268.00	62.90	66.87
264.00	60.20	59.68
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF121416\
Data File : BF091611.D
Acq On : 15 Dec 2016 5:46
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 19 04:42:41 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF120916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 16 00:35:41 2016
Response via : Initial Calibration

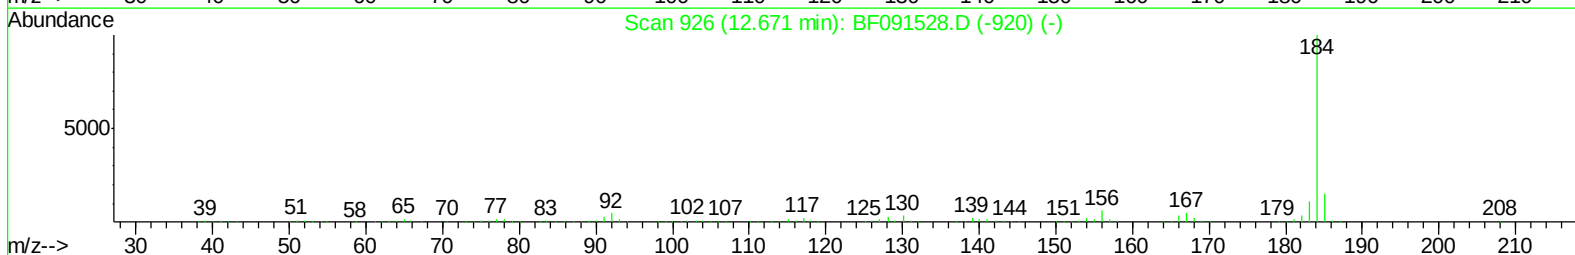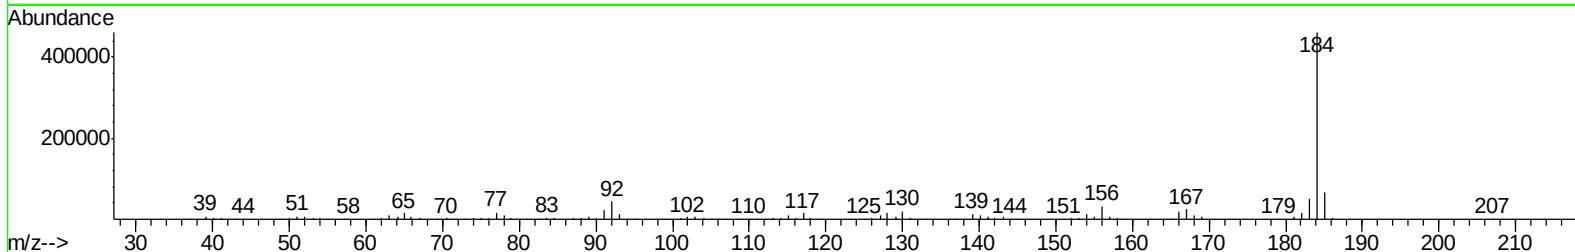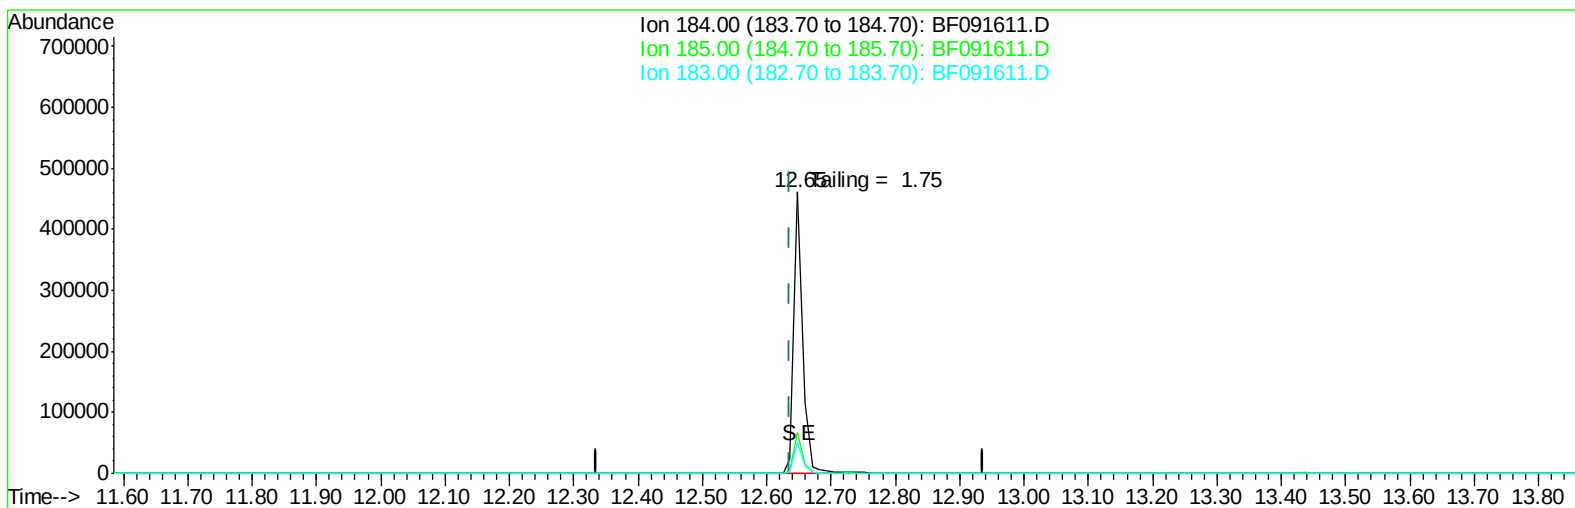

TIC: BF091611.D

(76) Benzidine

12.648min (+0.012) 17960.87ng

response 434288

Ion	Exp%	Act%
184.00	100	100
185.00	16.40	14.63
183.00	11.10	10.76
0.00	0.00	0.00