


Data Path : Z:\HPCHEM1\BNA F\DATA\BF121416\
 Data File : BF091577.D
 Acq On : 14 Dec 2016 10:31
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF120916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 09 19:00:21 2016

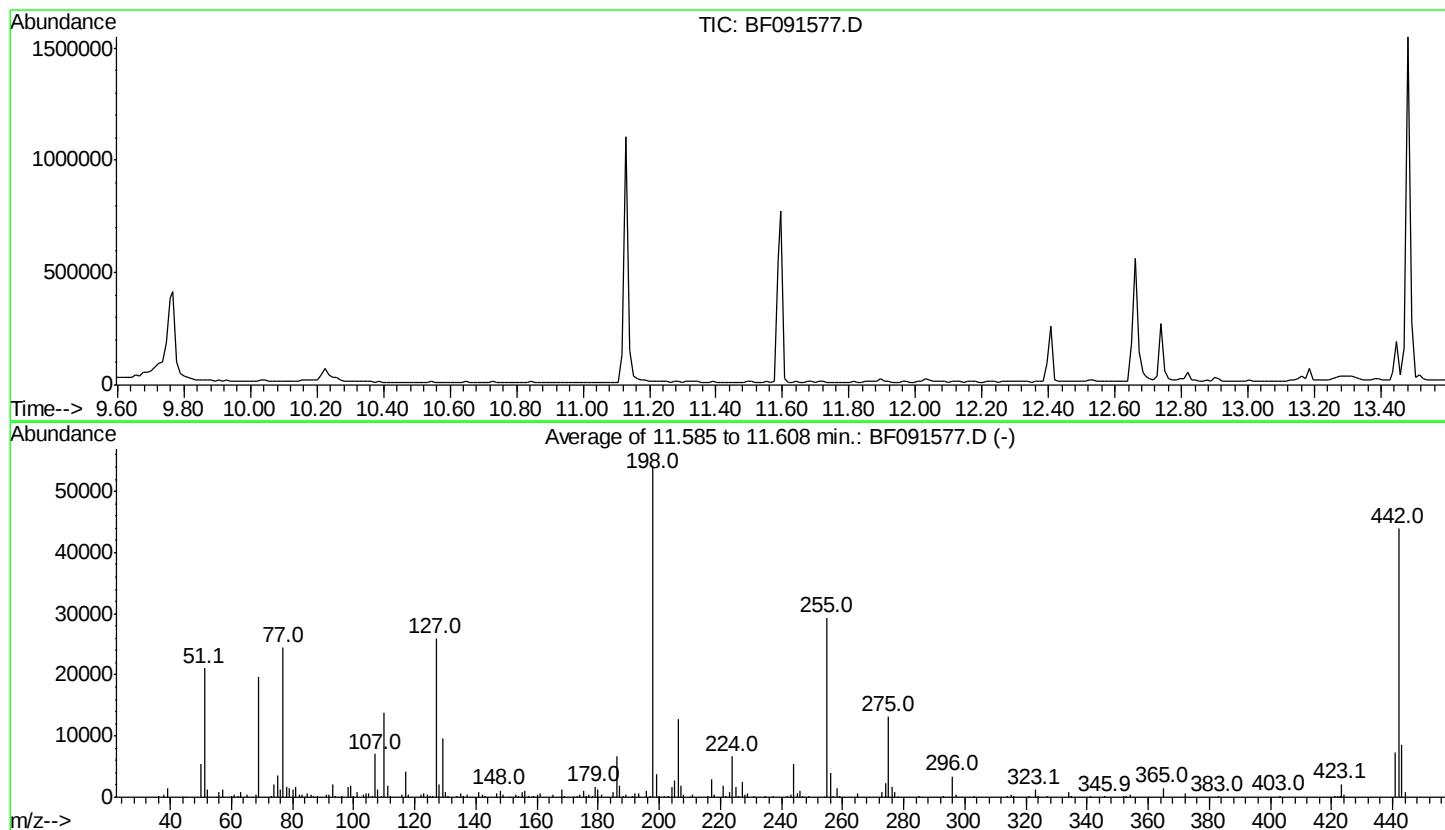

AutoFind: Scans 831, 832, 833; Background Corrected with Scan 828

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.9	21081	PASS
68	69	0.00	2	1.7	325	PASS
69	198	0.00	100	36.3	19688	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.7	25853	PASS
197	198	0.00	2	0.4	205	PASS
198	198	100	100	100.0	54205	PASS
199	198	5	9	6.9	3731	PASS
275	198	10	60	24.2	13132	PASS
365	198	1	100	2.8	1497	PASS
441	442	0.01	24	16.5	7243	PASS
442	198	50	100	81.0	43880	PASS
443	442	15	24	19.3	8483	PASS