


Data Path : Z:\HPCHEM1\BNA F\DATA\BF121416\
 Data File : BF091586.D
 Acq On : 14 Dec 2016 16:10
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF120916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 09 19:00:21 2016

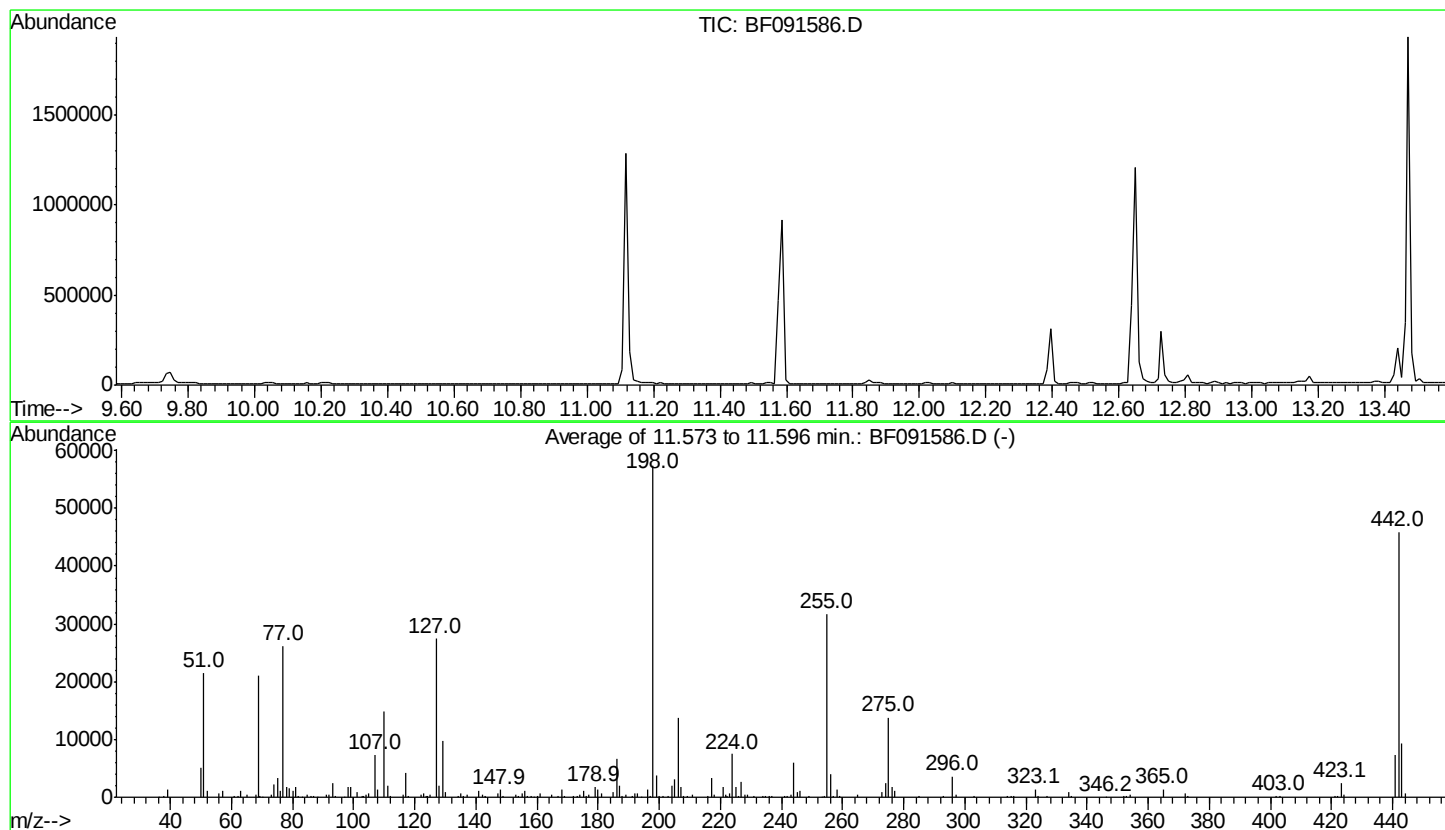

AutoFind: Scans 830, 831, 832; Background Corrected with Scan 827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.5	21499	PASS
68	69	0.00	2	1.9	396	PASS
69	198	0.00	100	36.7	21078	PASS
70	69	0.00	2	0.5	101	PASS
127	198	10	80	47.8	27453	PASS
197	198	0.00	2	0.5	269	PASS
198	198	100	100	100.0	57397	PASS
199	198	5	9	6.4	3689	PASS
275	198	10	60	24.0	13757	PASS
365	198	1	100	2.5	1435	PASS
441	442	0.01	24	16.0	7341	PASS
442	198	50	100	80.1	45972	PASS
443	442	15	24	20.3	9335	PASS