


Data Path : Z:\HPCHEM1\BNA F\DATA\BF121416\
Data File : BF091611.D
Acq On : 15 Dec 2016 5:46
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF120916.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Dec 09 19:00:21 2016

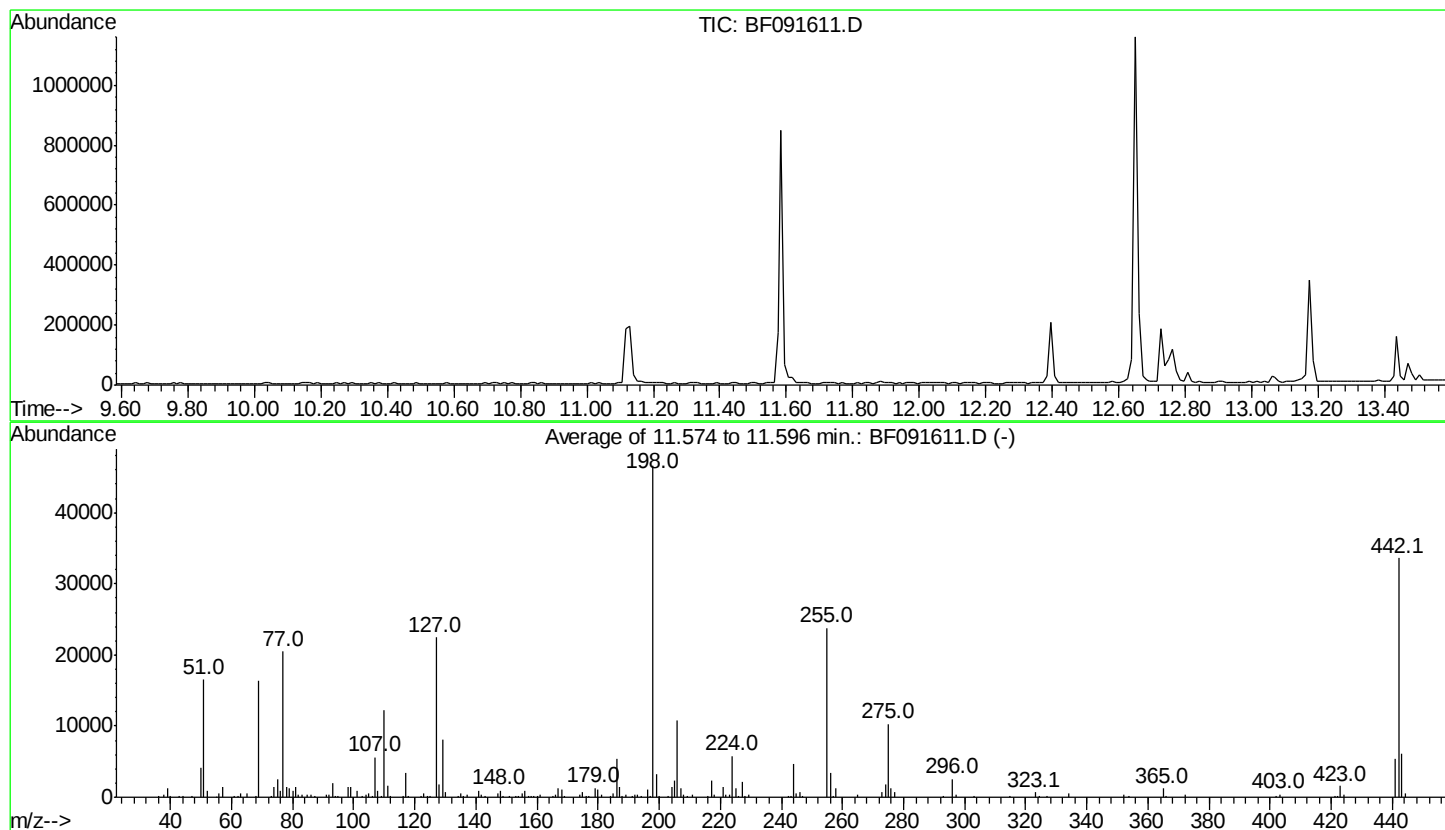

AutoFind: Scans 830, 831, 832; Background Corrected with Scan 827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.5	16526	PASS
68	69	0.00	2	1.1	175	PASS
69	198	0.00	100	35.2	16418	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.1	22410	PASS
197	198	0.00	2	0.5	224	PASS
198	198	100	100	100.0	46605	PASS
199	198	5	9	7.1	3307	PASS
275	198	10	60	22.1	10310	PASS
365	198	1	100	2.6	1214	PASS
441	442	0.01	24	16.1	5413	PASS
442	198	50	100	72.2	33629	PASS
443	442	15	24	18.4	6186	PASS