




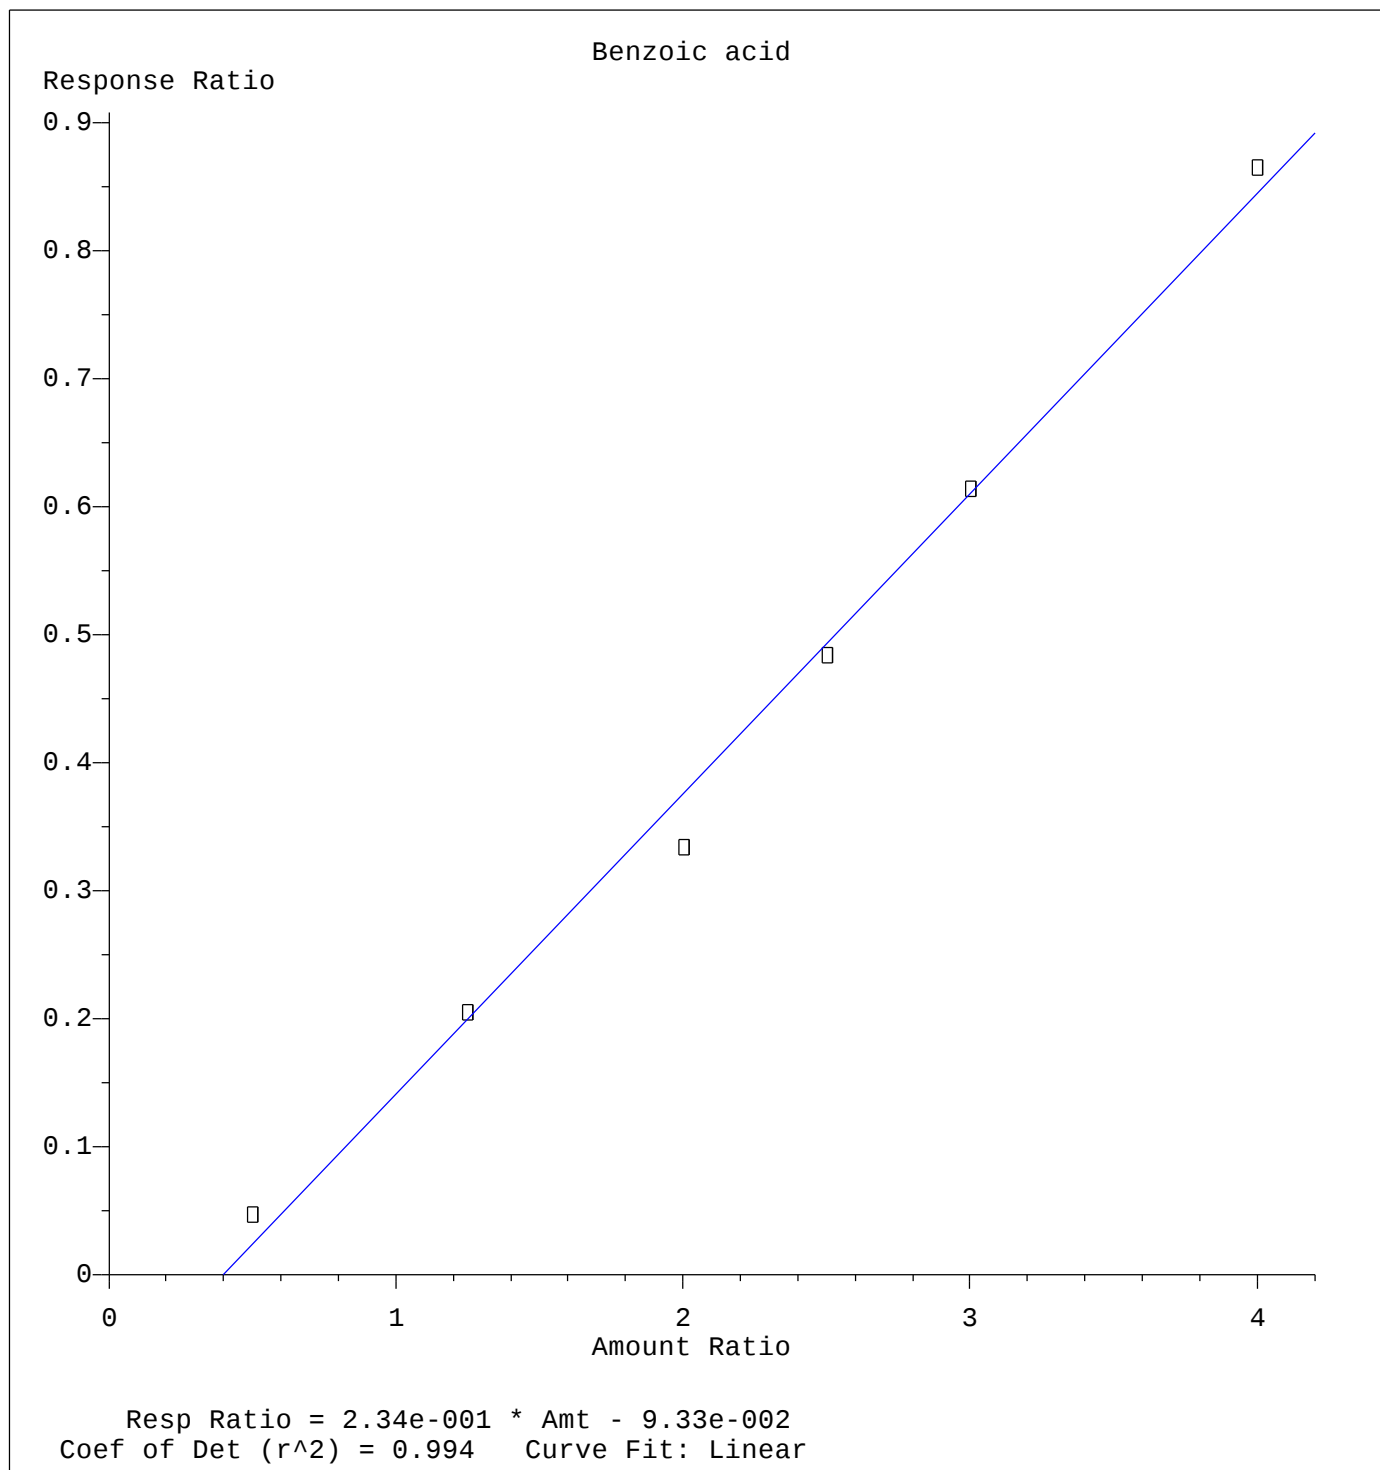


Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
Calibration Table Last Updated: Thu Dec 14 15:42:32 2017

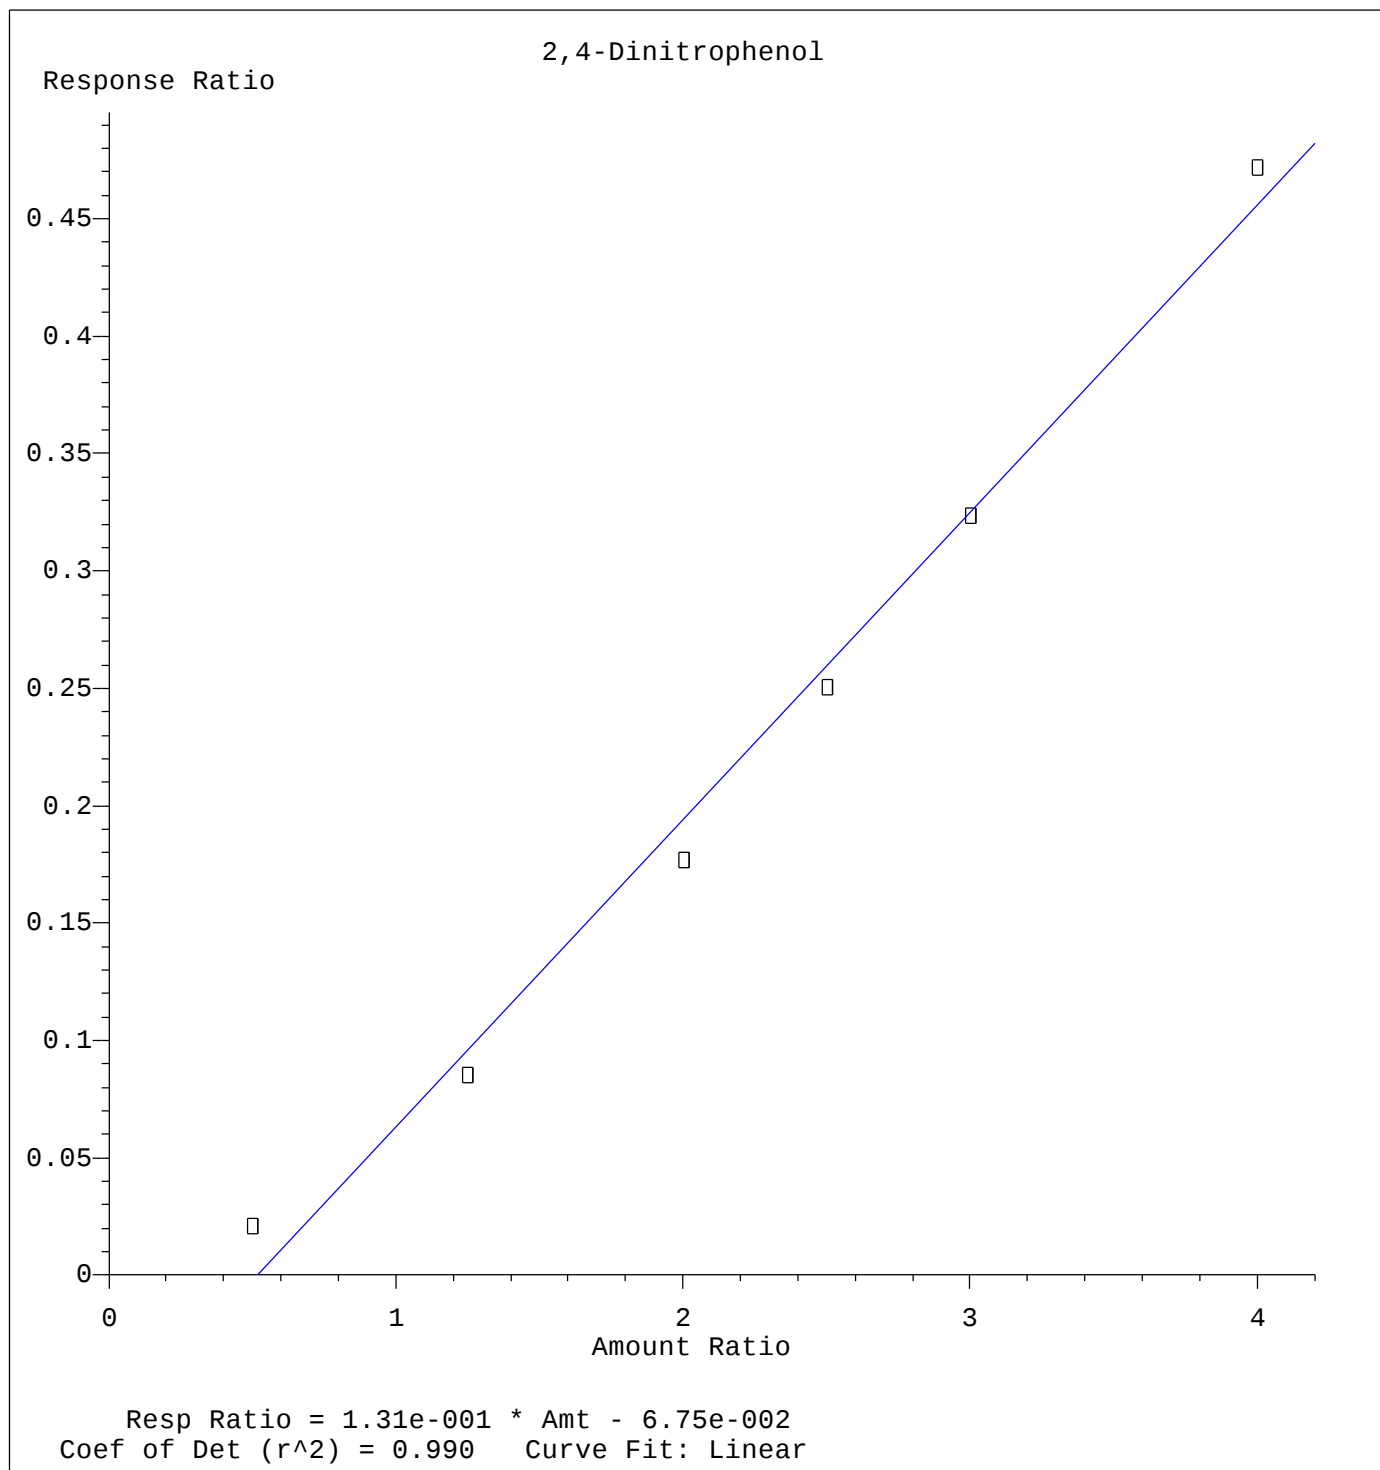

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
Calibration Table Last Updated: Thu Dec 14 15:42:32 2017

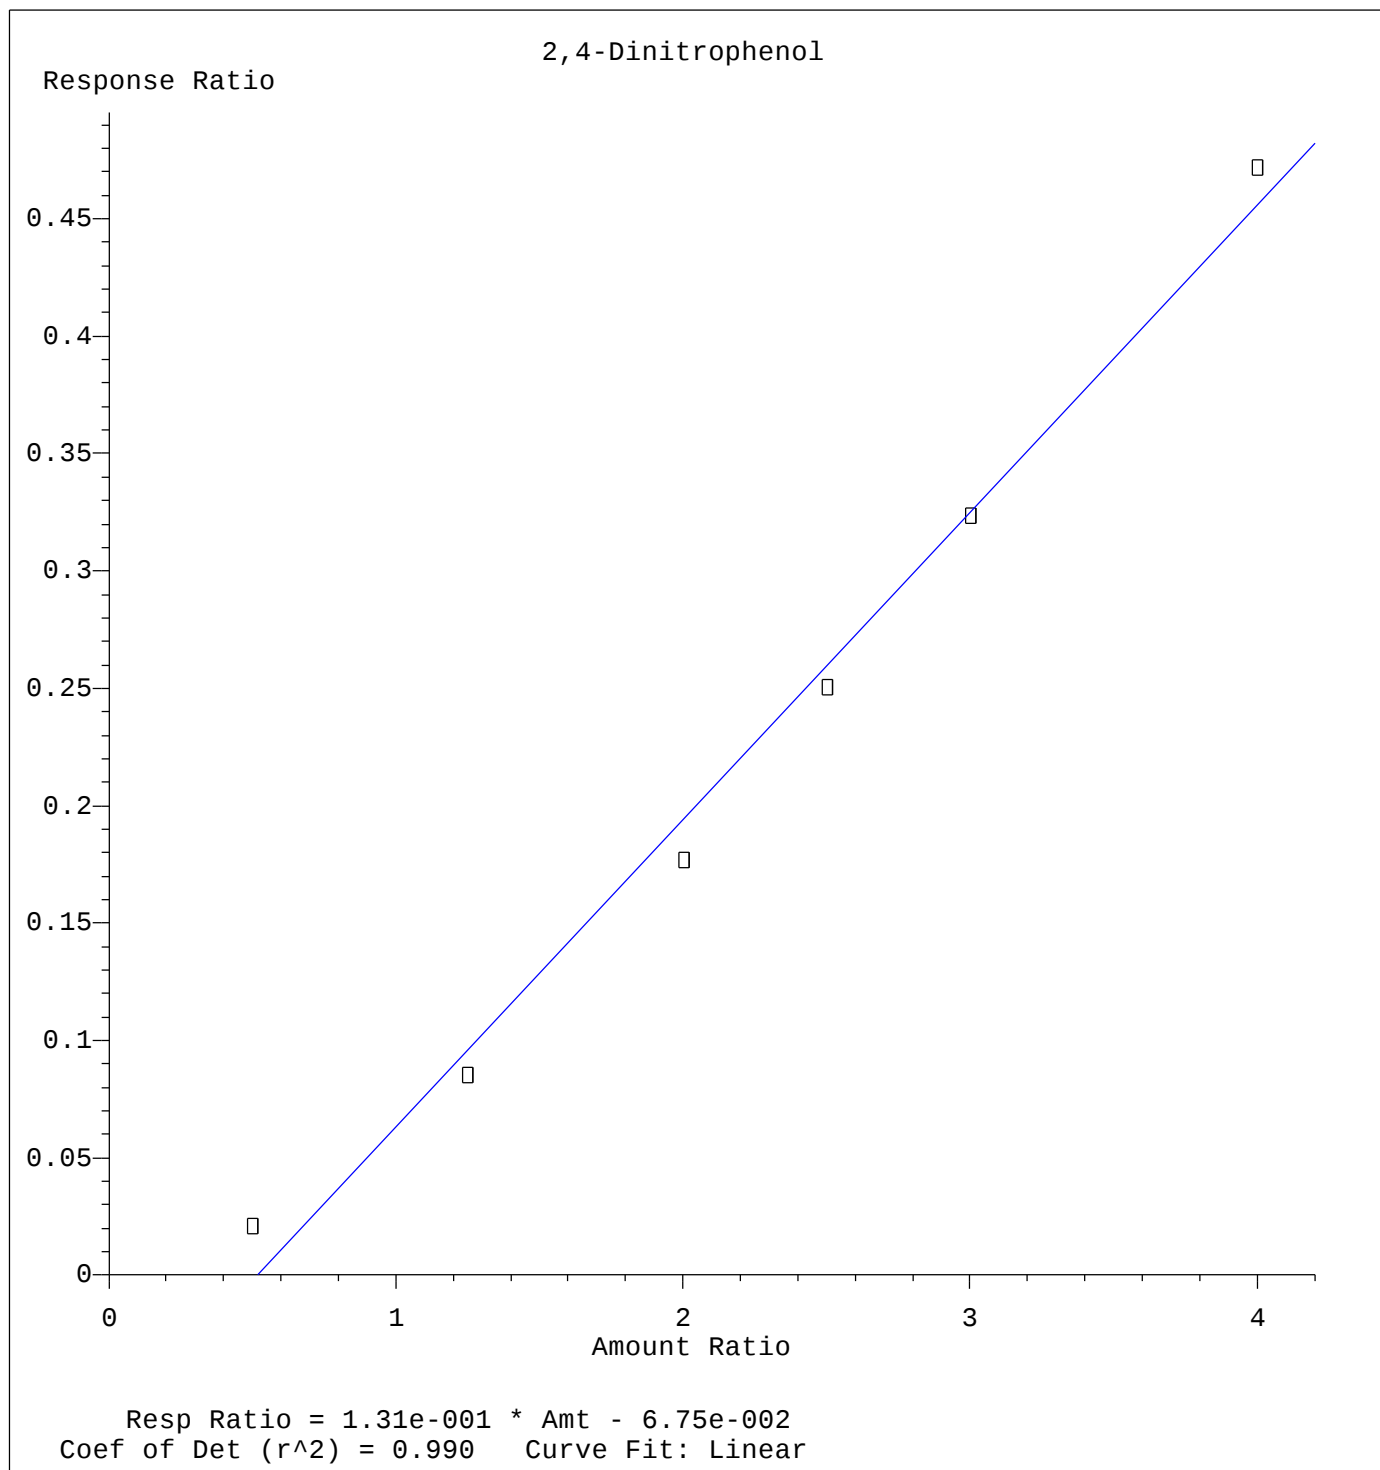


Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
Calibration Table Last Updated: Thu Dec 14 15:42:32 2017

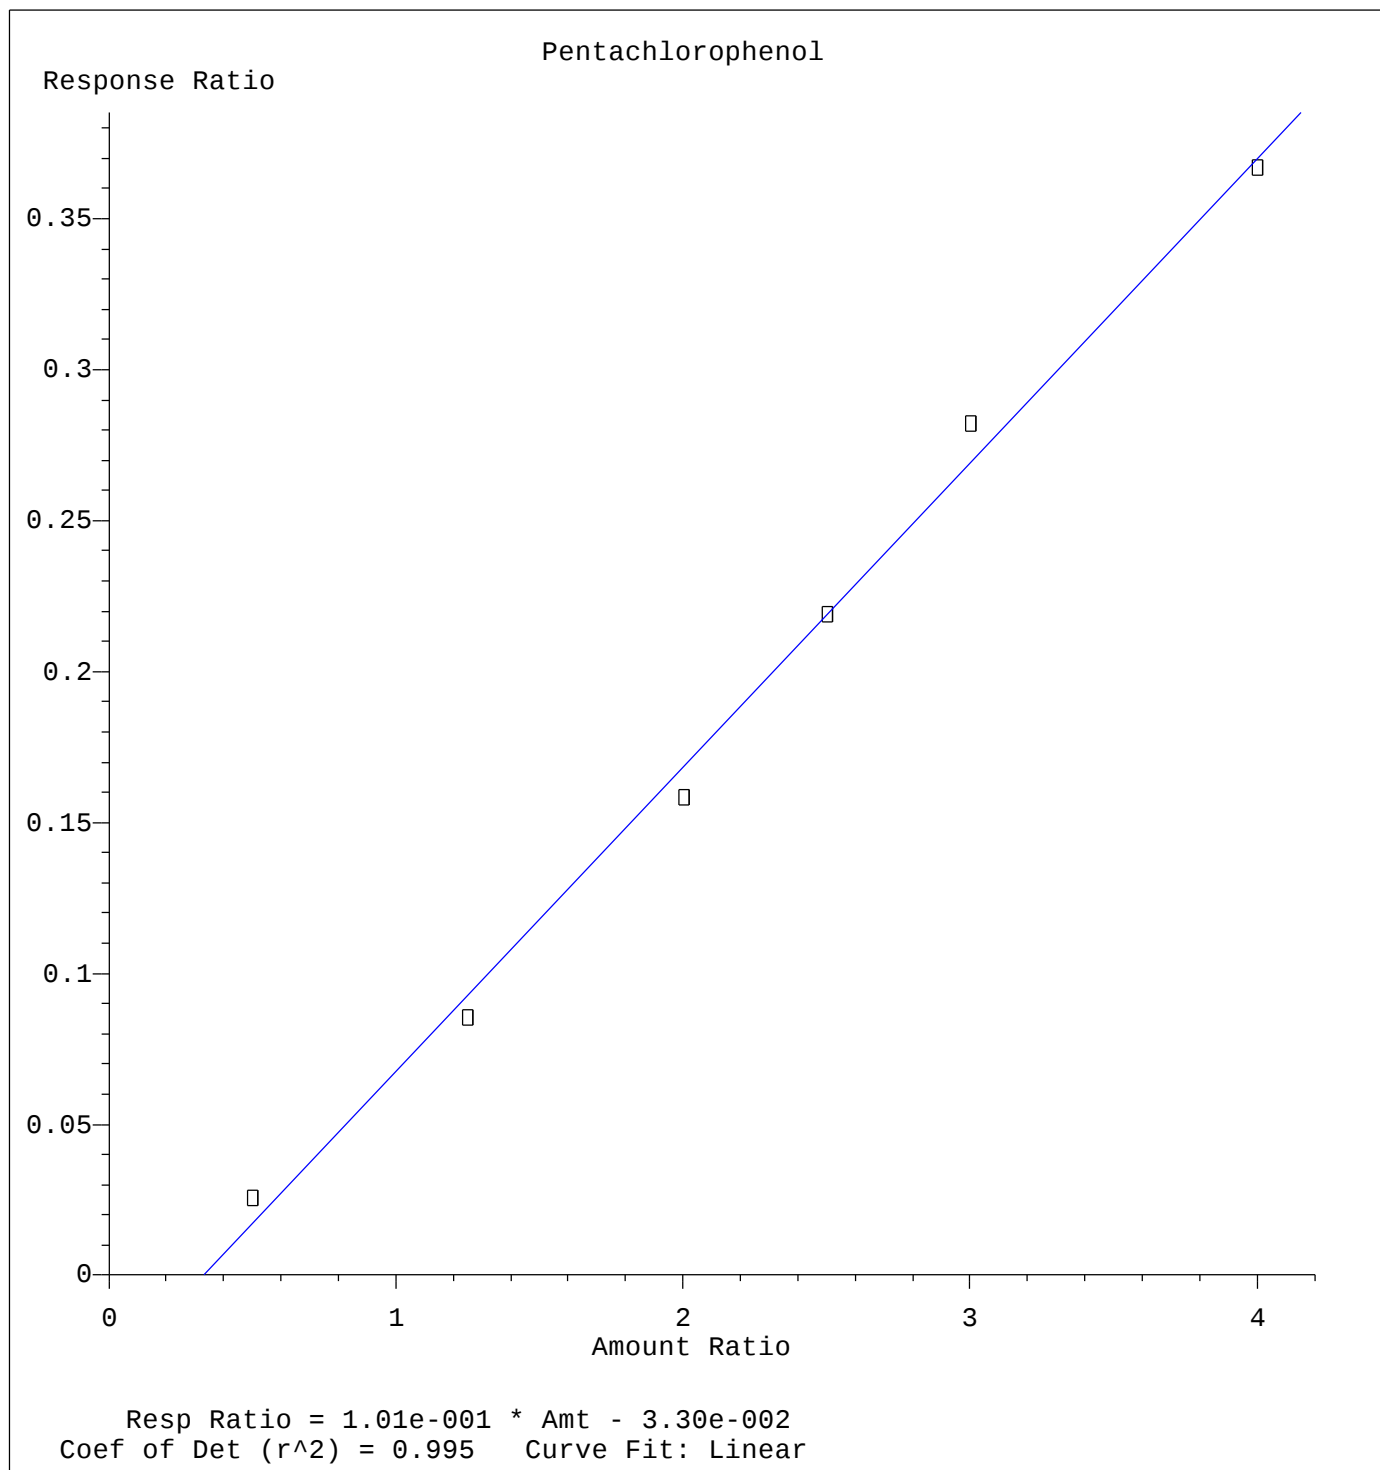

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
Calibration Table Last Updated: Thu Dec 14 15:42:32 2017

Hexachlorocyclopentadiene

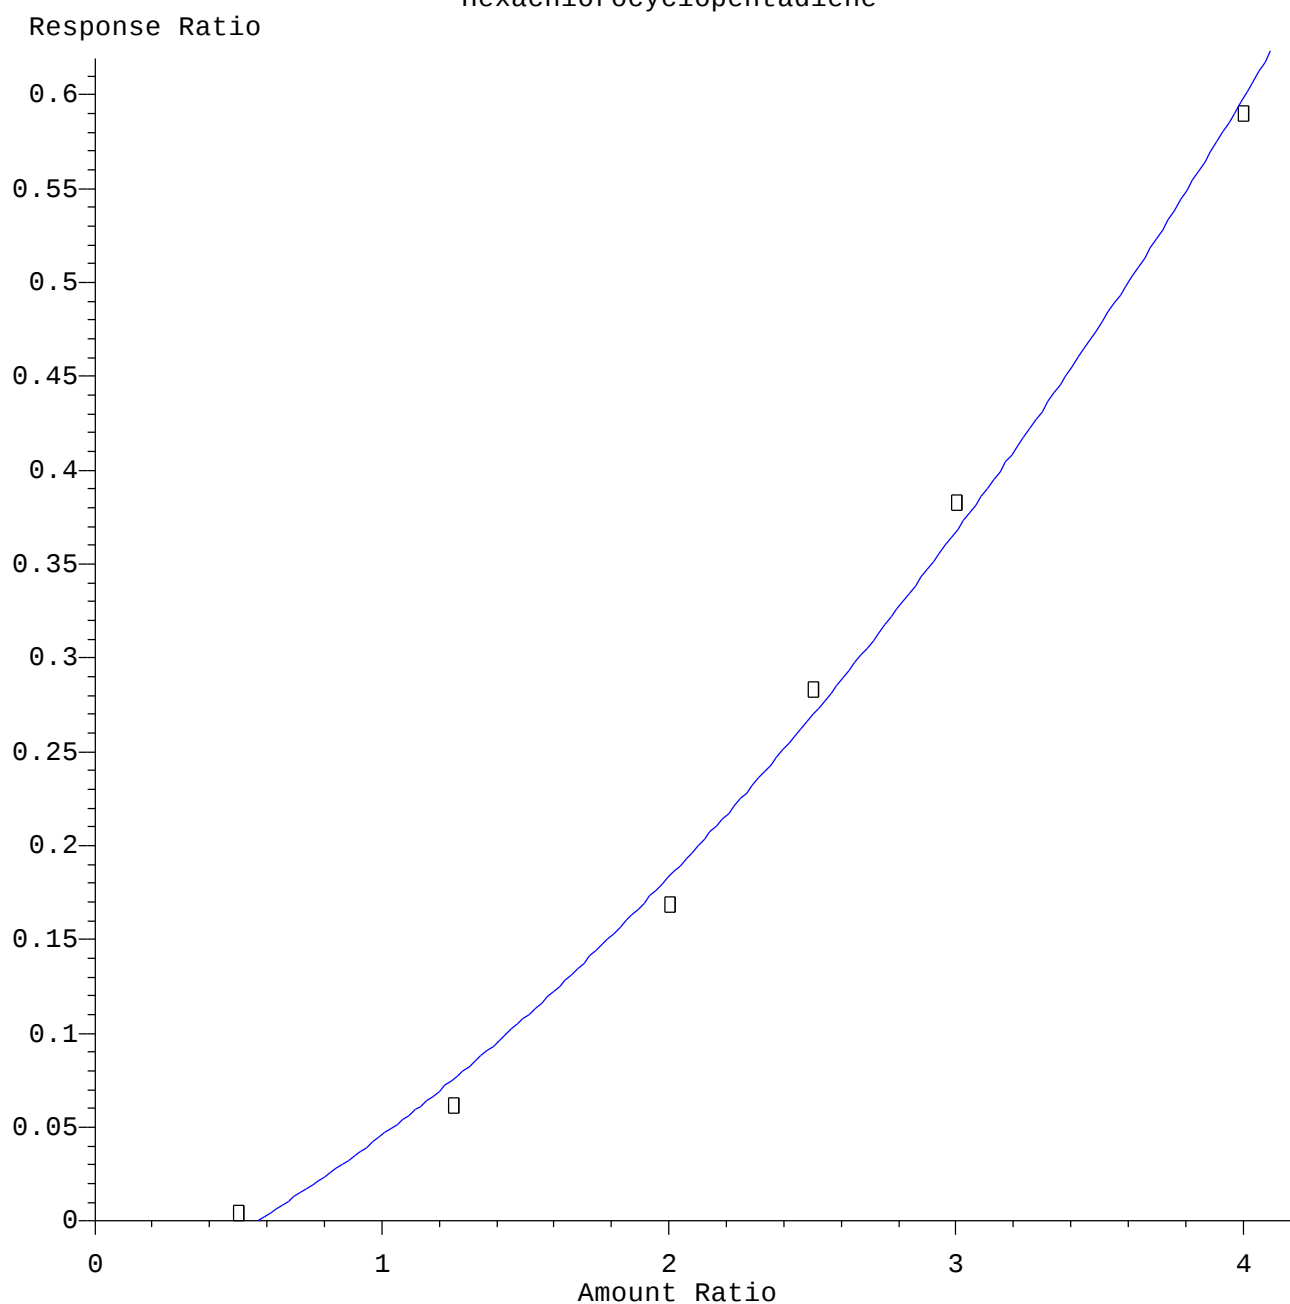

$R = 2.32e-002 A^2 + 6.84e-002 A - 4.60e-002$
Coef of Det (r^2) = 0.996 Curve Fit: Quadratic

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
Calibration Table Last Updated: Thu Dec 14 15:42:32 2017