
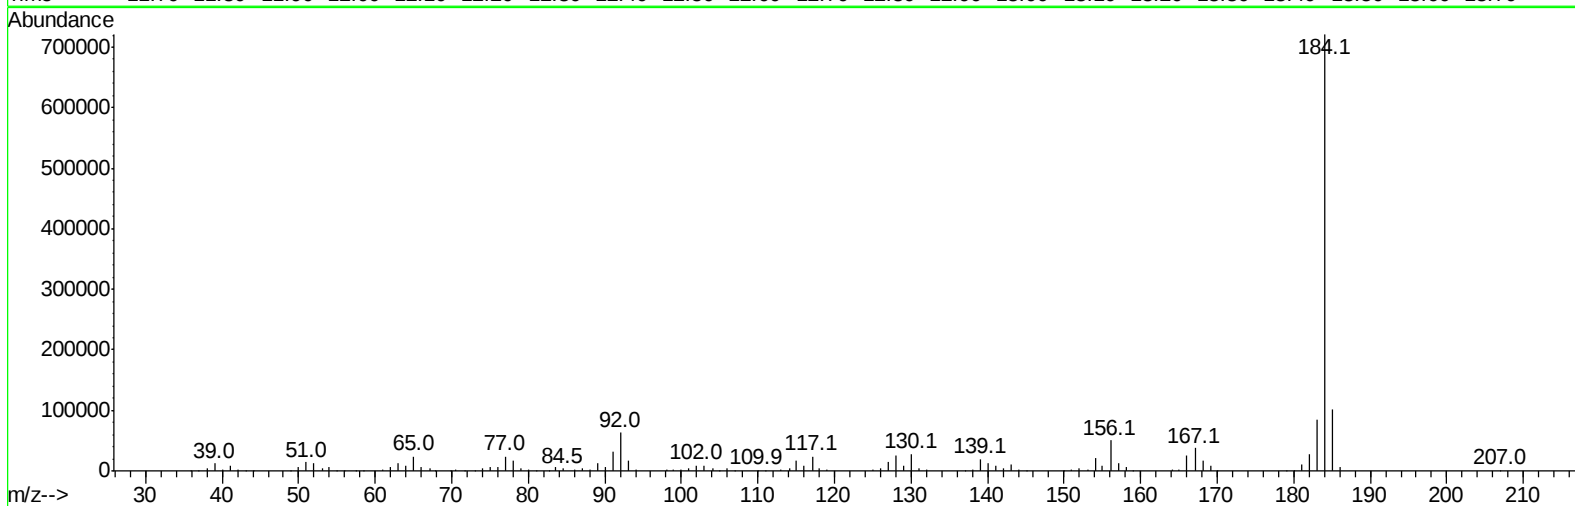


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF121417\
Data File : BF101386.D
Acq On : 14 Dec 2017 10:36
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 15 05:55:12 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 14 15:42:32 2017
Response via : Initial Calibration

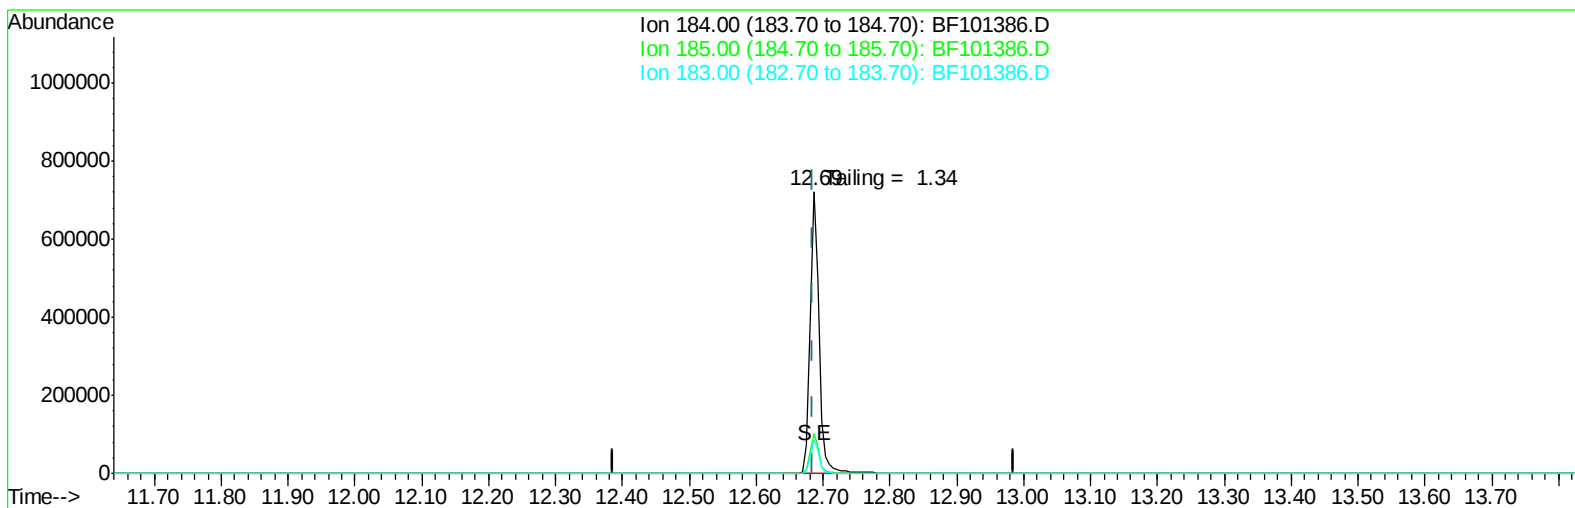

TIC: BF101386.D

(76) Benzidine



12.686min (-0.000) 0.00ng

response 686099

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.20
183.00	11.60	11.77
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF121417\
Data File : BF101386.D
Acq On : 14 Dec 2017 10:36
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 15 05:55:12 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 14 15:42:32 2017
Response via : Initial Calibration

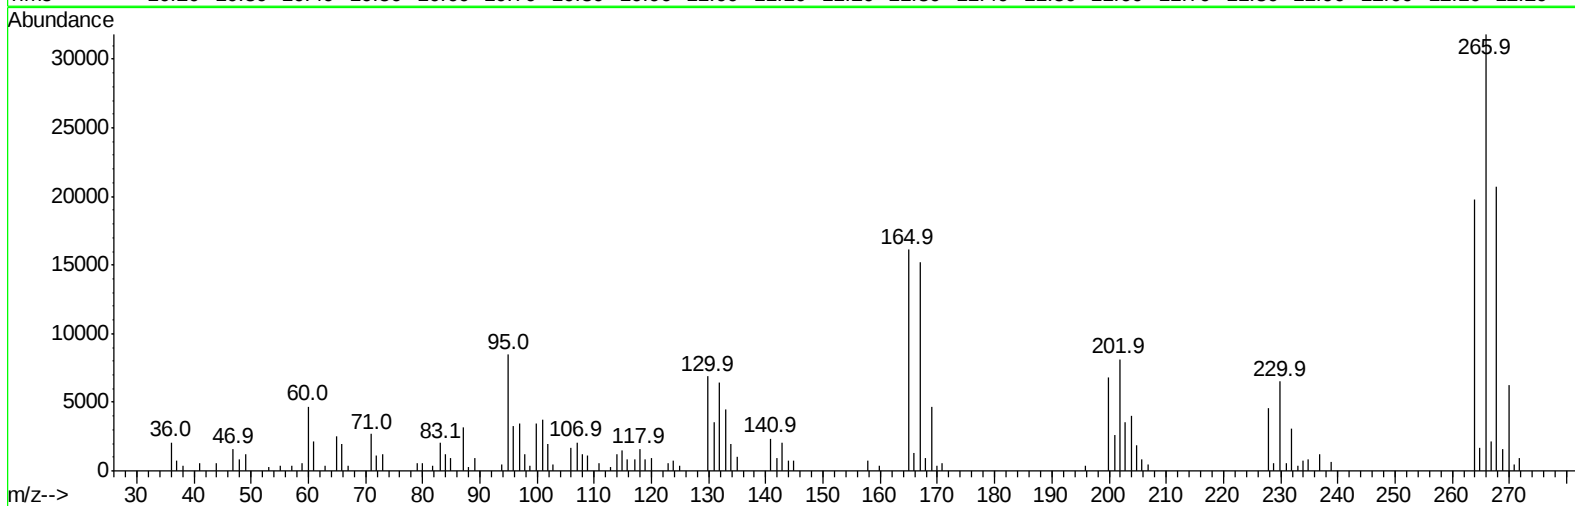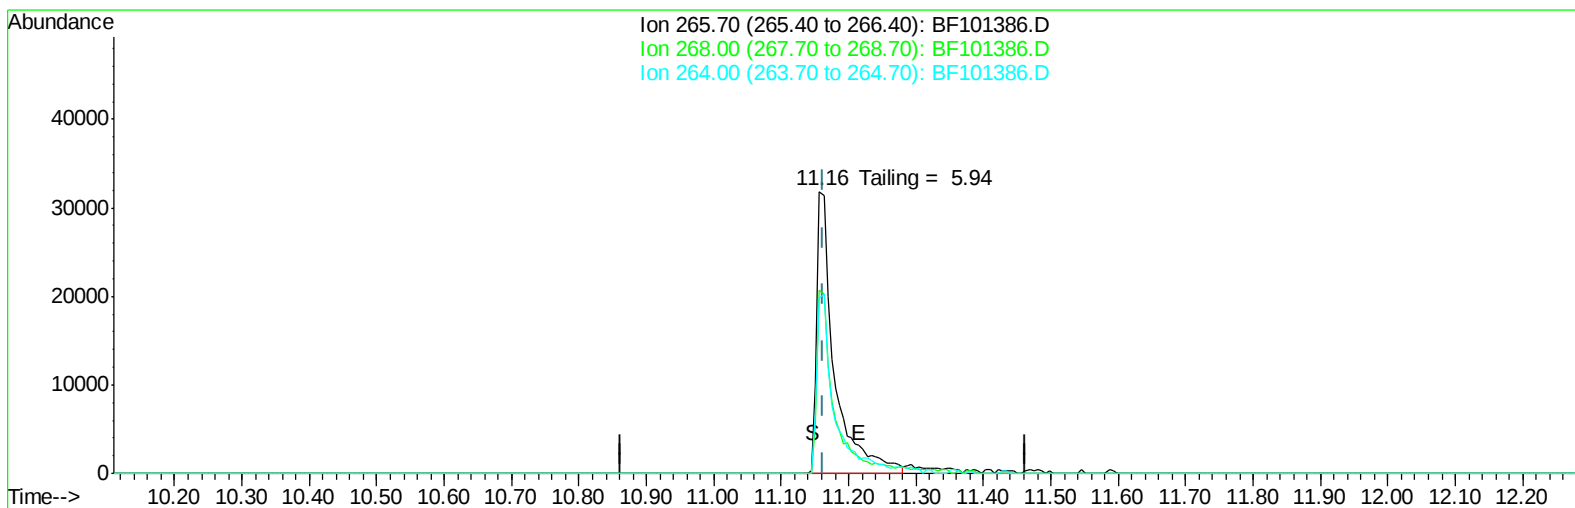

TIC: BF101386.D

(69) Pentachlorophenol (C)

11.157min (-0.005) 25274.99ng

response 57025

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	65.12
264.00	61.90	62.32
0.00	0.00	0.00