
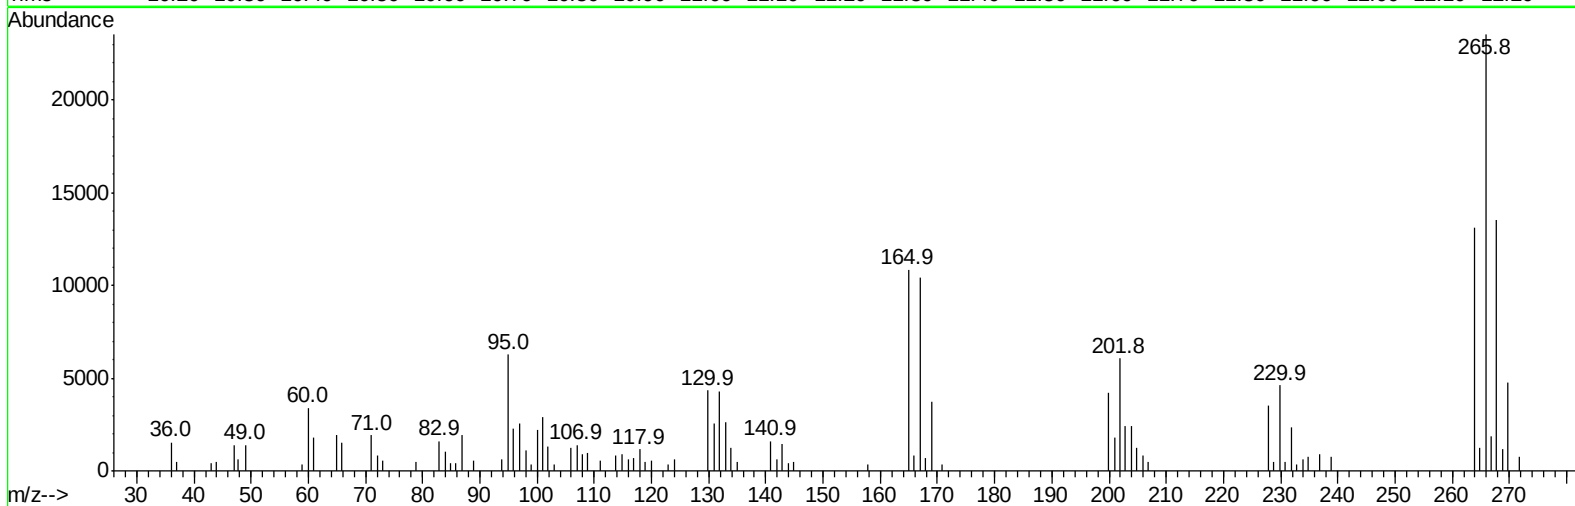


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF121417\
Data File : BF101423.D
Acq On : 15 Dec 2017 5:10
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 15 05:59:31 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 14 15:42:32 2017
Response via : Initial Calibration

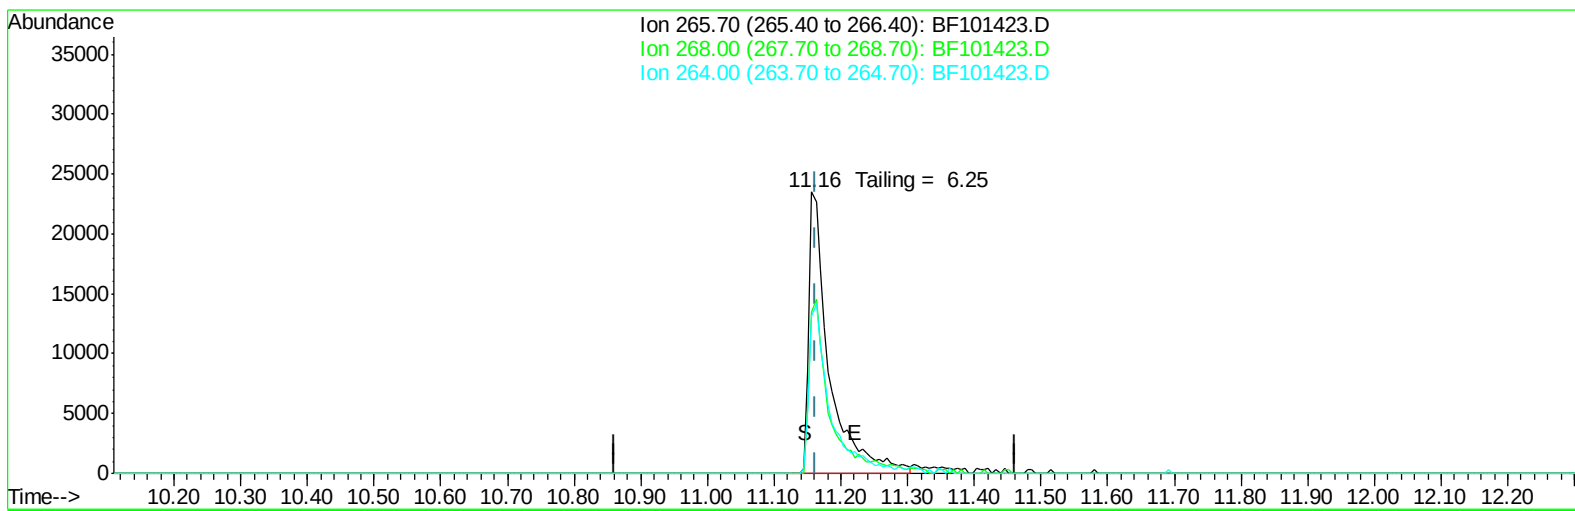

TIC: BF101423.D

(69) Pentachlorophenol (C)



11.157min (-0.005) 30594.09ng

response 48536

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	57.41
264.00	61.90	55.84
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF121417\
Data File : BF101423.D
Acq On : 15 Dec 2017 5:10
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 15 05:59:31 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 14 15:42:32 2017
Response via : Initial Calibration

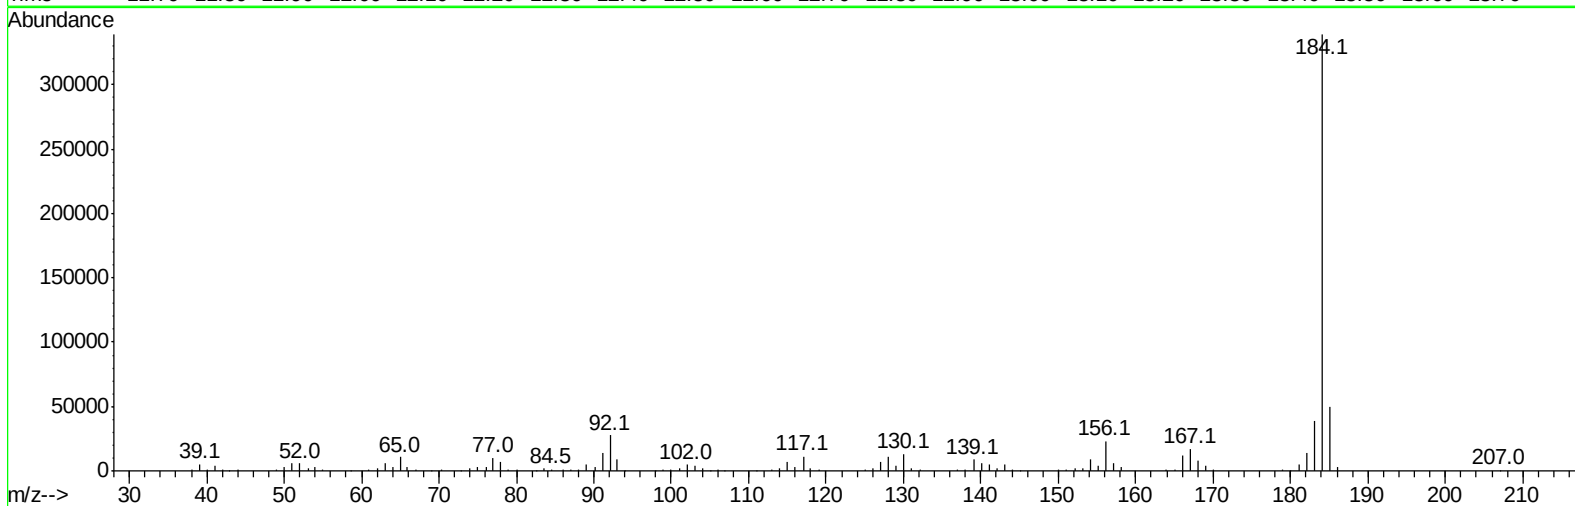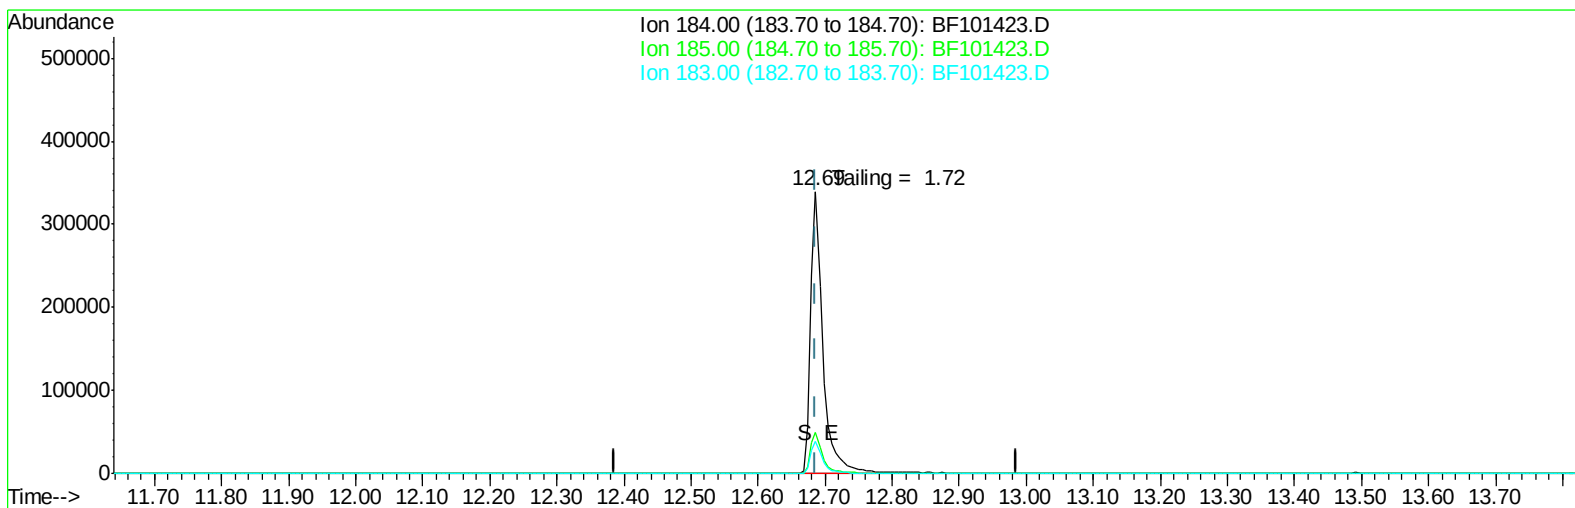

TIC: BF101423.D

(76) Benzidine

12.686min (-0.000) 0.00ng

response 413414

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.78
183.00	11.60	11.57
0.00	0.00	0.00