


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA F\Data\BF121417\
 Data File : BF101396.D
 Acq On : 14 Dec 2017 16:25
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 14 15:42:32 2017

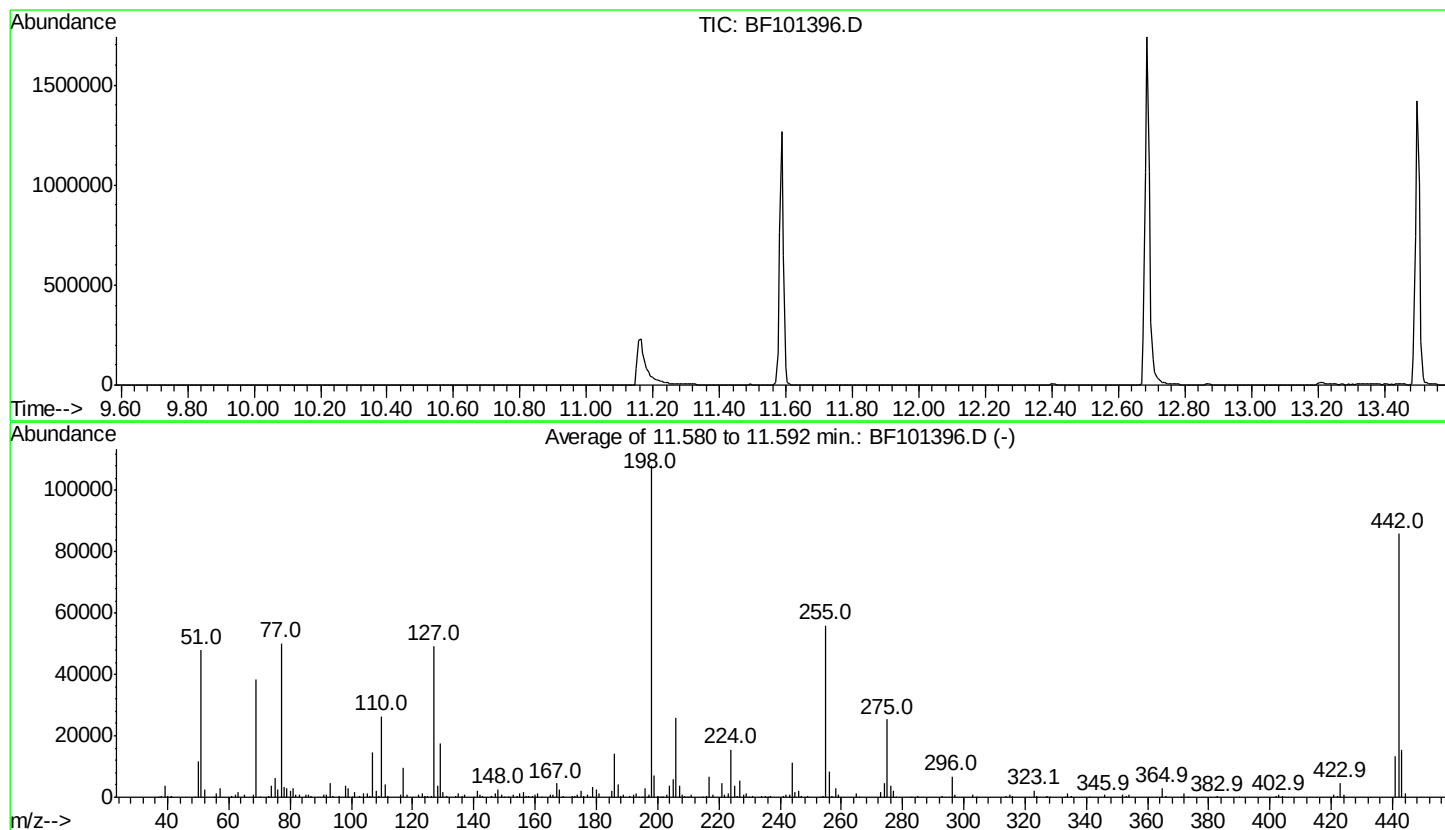

AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.5	48133	PASS
68	69	0.00	2	1.8	677	PASS
69	198	0.00	100	35.6	38474	PASS
70	69	0.00	2	0.4	135	PASS
127	198	10	80	45.6	49288	PASS
197	198	0.00	2	0.7	742	PASS
198	198	100	100	100.0	108058	PASS
199	198	5	9	6.6	7082	PASS
275	198	10	60	23.4	25274	PASS
365	198	1	100	2.8	3031	PASS
441	443	0.01	100	85.5	13357	PASS
442	198	50	100	79.5	85858	PASS
443	442	15	24	18.2	15628	PASS